

SUPERVISOR TEST




AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 05/01/2023

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:45
INTERNAL STANDARD	VERIFIED	07:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:46
BLANK TEST	0.00	07:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:47
BLANK TEST	0.00	07:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:48
BLANK TEST	0.00	07:49

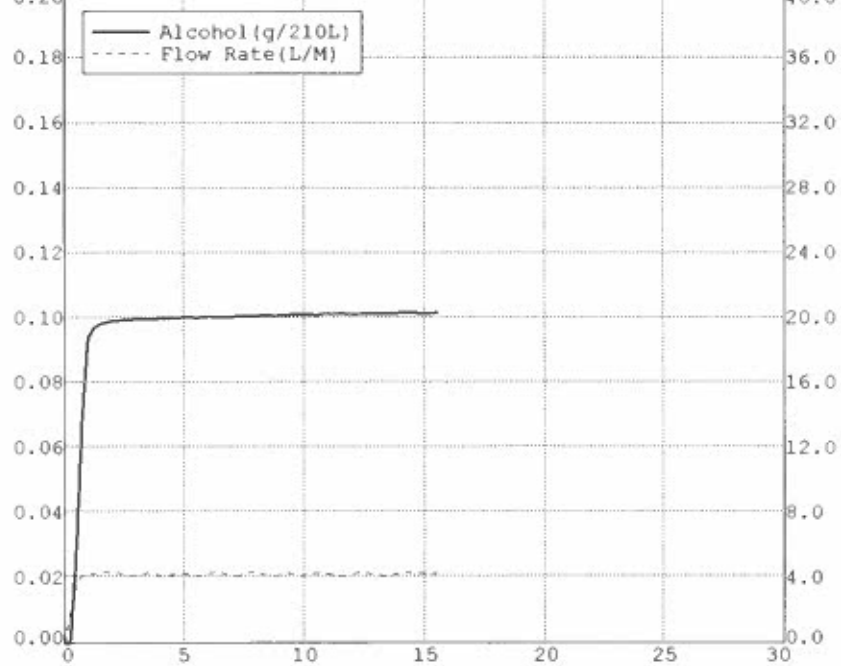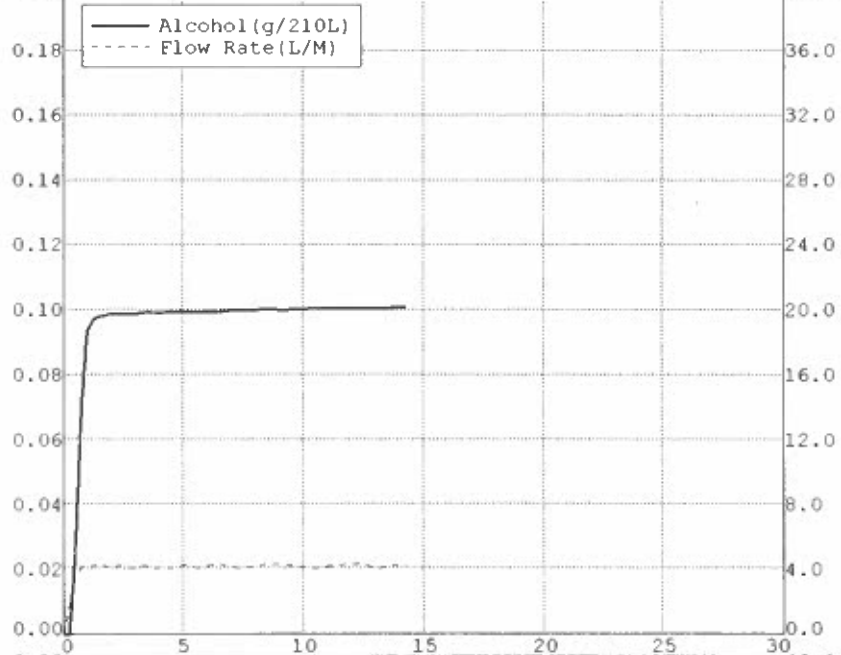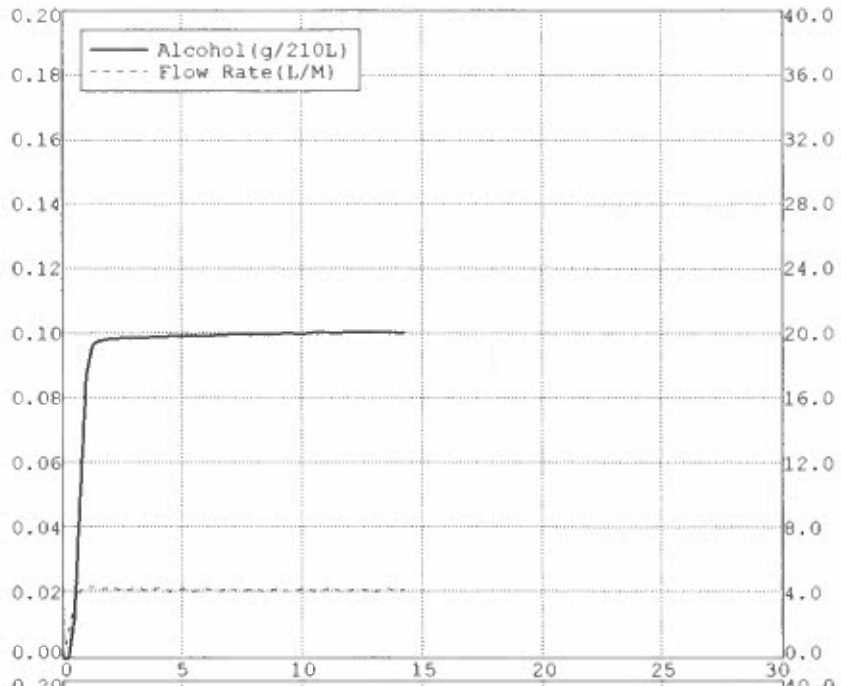

SOLUTION CHANGE

AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 05/01/2023

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:09
INTERNAL STANDARD	VERIFIED	08:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	08:10
BLANK TEST	0.00	08:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:11
BLANK TEST	0.00	08:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:12
BLANK TEST	0.00	08:13

