

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 10/02/2023

OPERATOR NAME: GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:13
INTERNAL STANDARD	VERIFIED	07:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:13
BLANK TEST	0.00	07:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:15
BLANK TEST	0.00	07:16
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	07:16
BLANK TEST	0.00	07:17

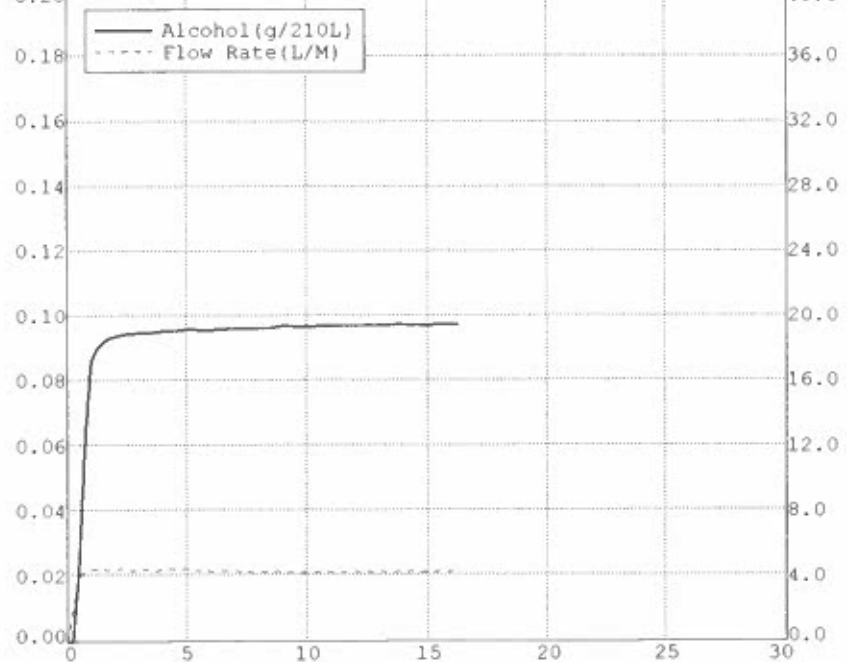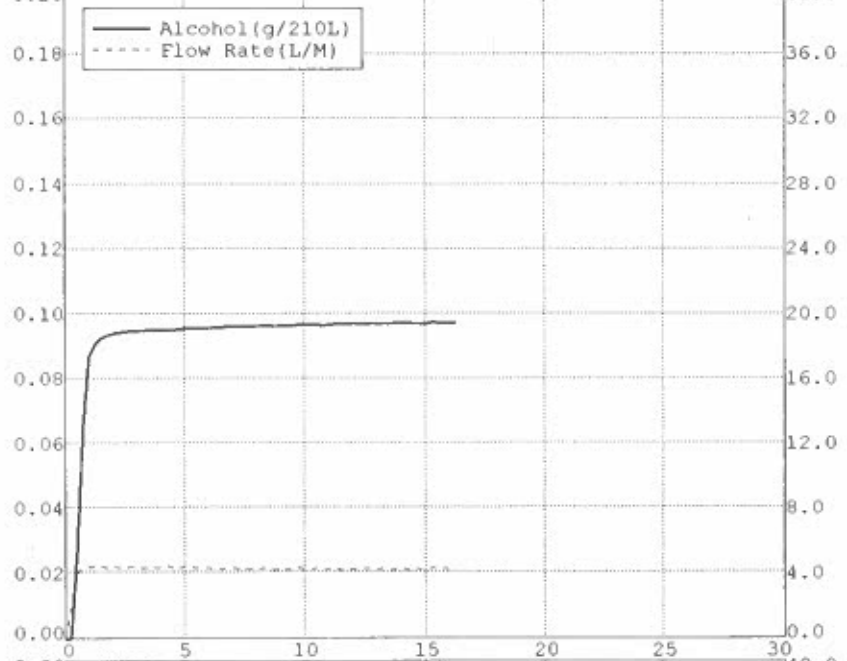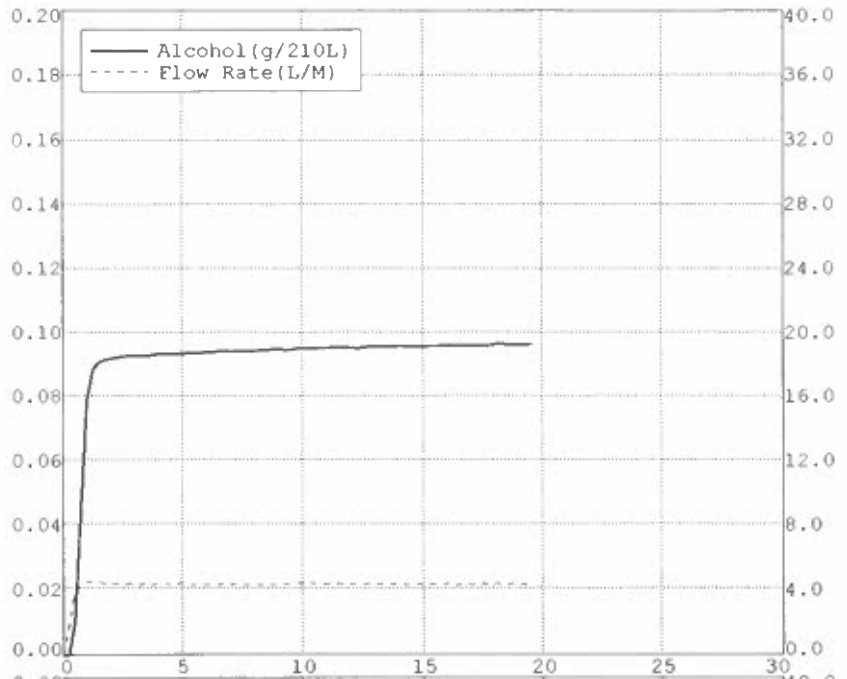

SOLUTION CHANGE

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 10/02/2023

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:08
INTERNAL STANDARD	VERIFIED	09:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:09
BLANK TEST	0.00	09:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:10
BLANK TEST	0.00	09:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:11
BLANK TEST	0.00	09:12

