

SUPERVISOR TEST




AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 01/02/2024

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:41
INTERNAL STANDARD	VERIFIED	07:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:41
BLANK TEST	0.00	07:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:42
BLANK TEST	0.00	07:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:44
BLANK TEST	0.00	07:44

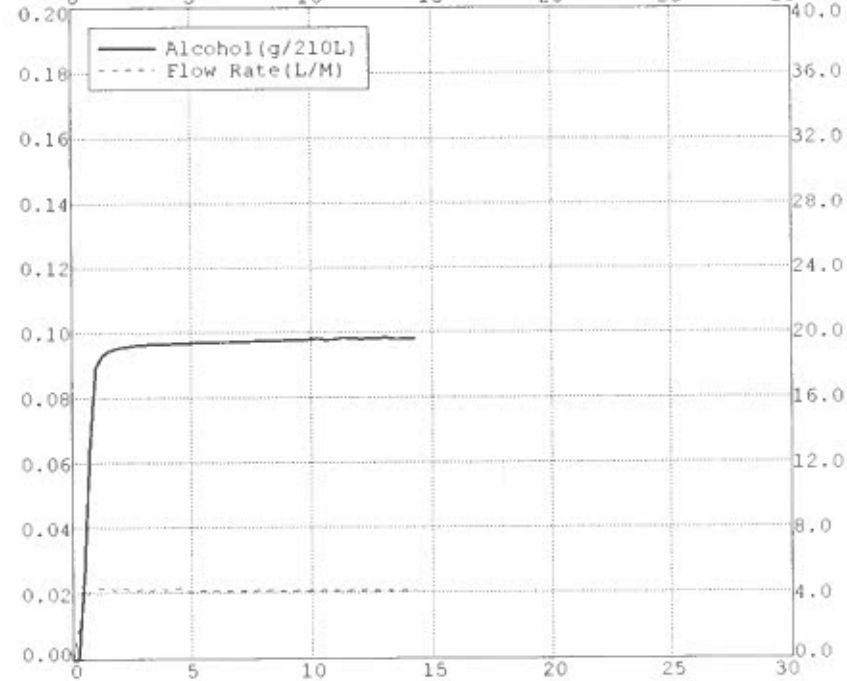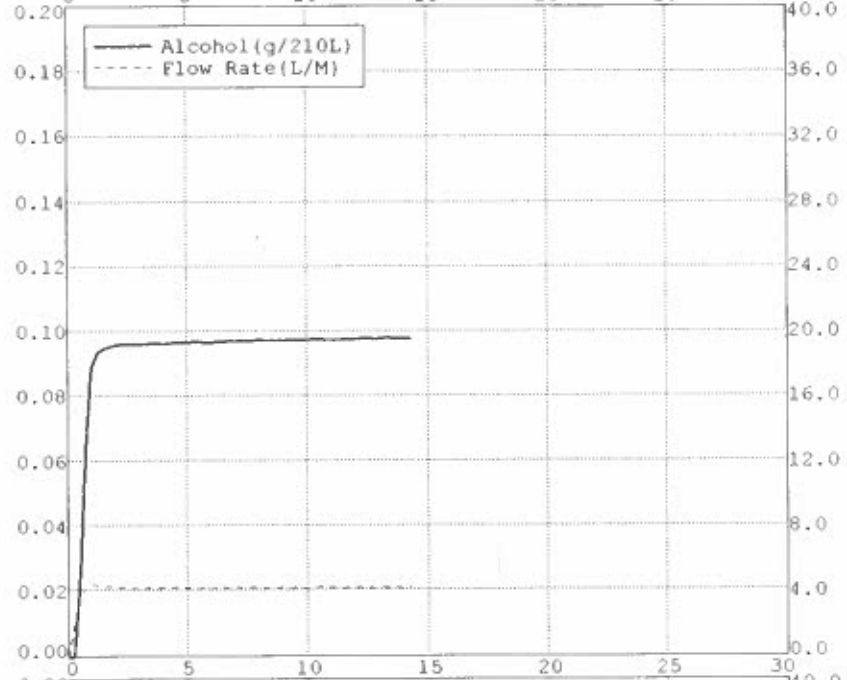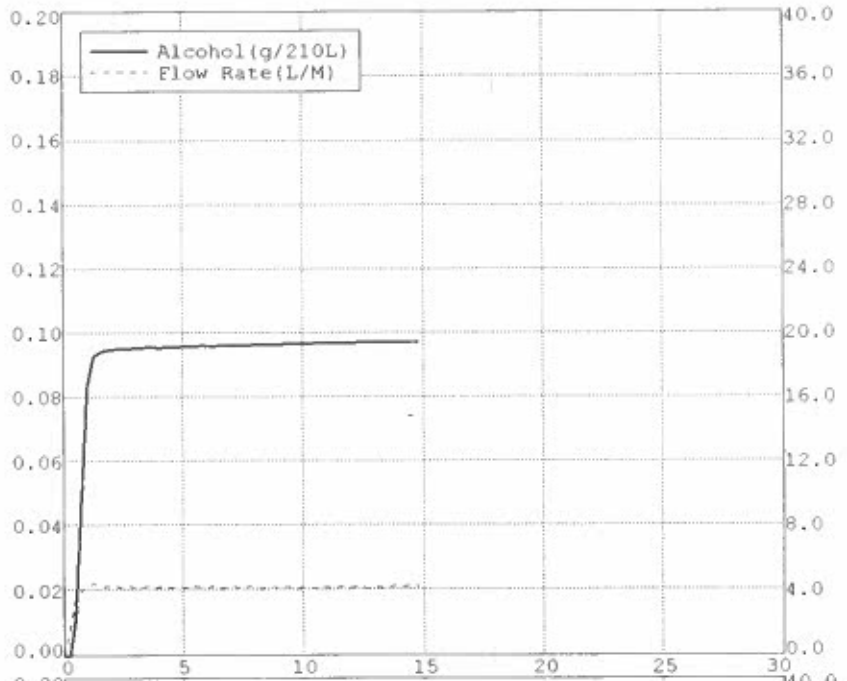

SOLUTION CHANGE

AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 01/02/2024

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:59
INTERNAL STANDARD	VERIFIED	12:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:00
BLANK TEST	0.00	13:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:01
BLANK TEST	0.00	13:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:02
BLANK TEST	0.00	13:03

