

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 02/01/2021

OPERATOR NAME: GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:45
INTERNAL STANDARD	VERIFIED	08:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:46
BLANK TEST	0.00	08:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:47
BLANK TEST	0.00	08:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:48
BLANK TEST	0.00	08:49

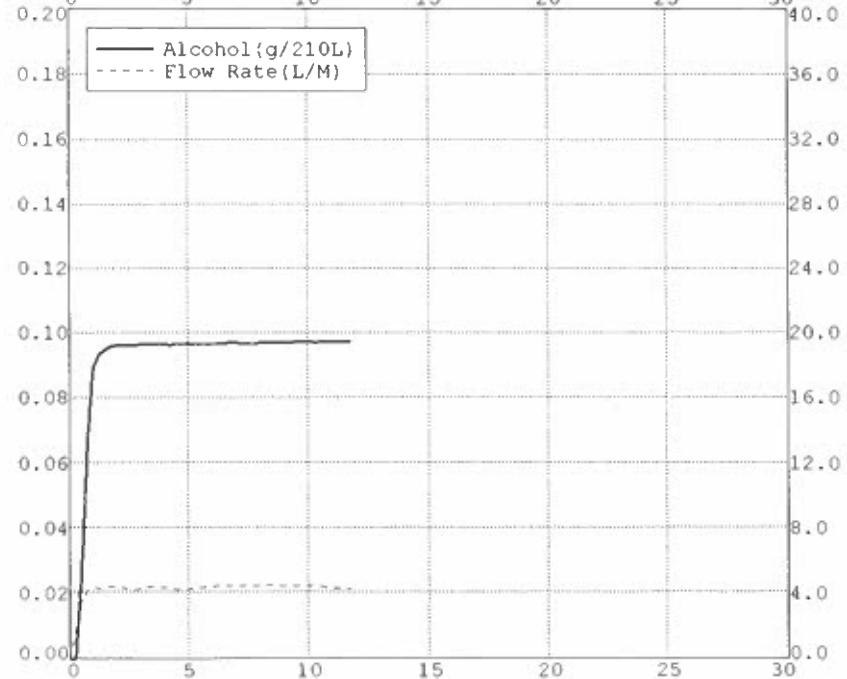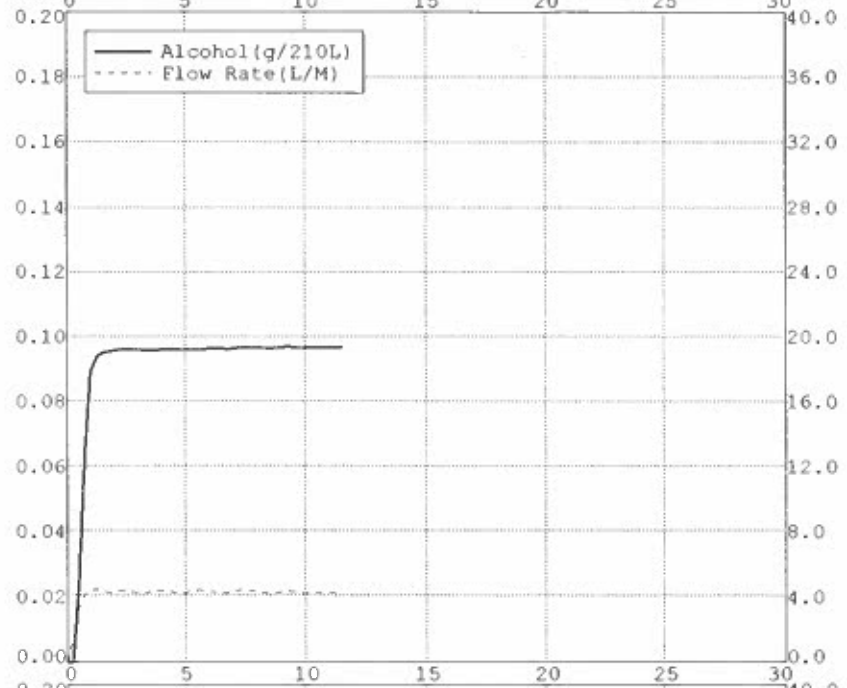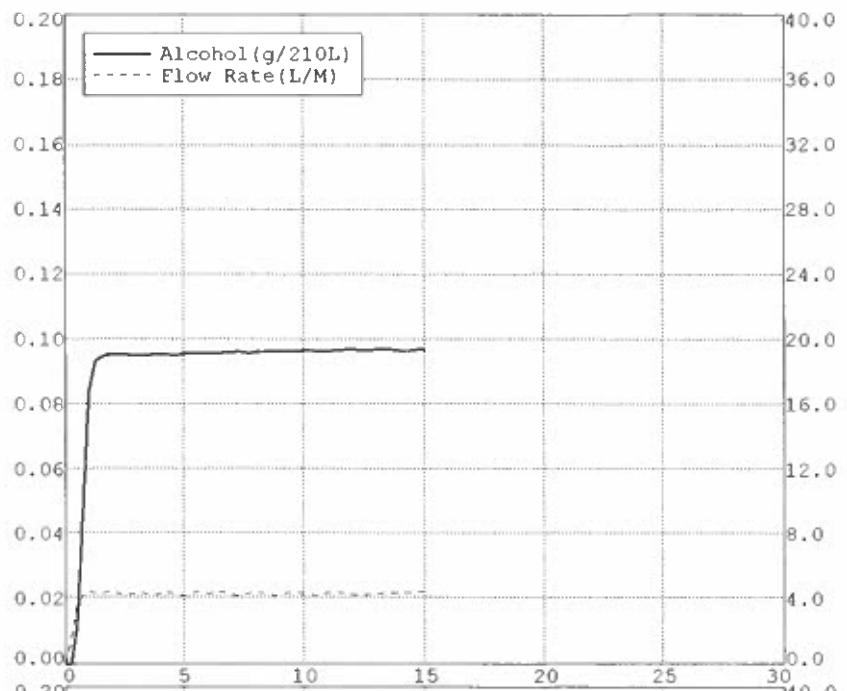

SOLUTION CHANGE

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 02/01/2021

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:24
INTERNAL STANDARD	VERIFIED	10:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:25
BLANK TEST	0.00	10:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:26
BLANK TEST	0.00	10:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:27
BLANK TEST	0.00	10:28

