

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 02/01/2022

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:23
INTERNAL STANDARD	VERIFIED	10:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:24
BLANK TEST	0.00	10:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:25
BLANK TEST	0.00	10:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:26
BLANK TEST	0.00	10:27

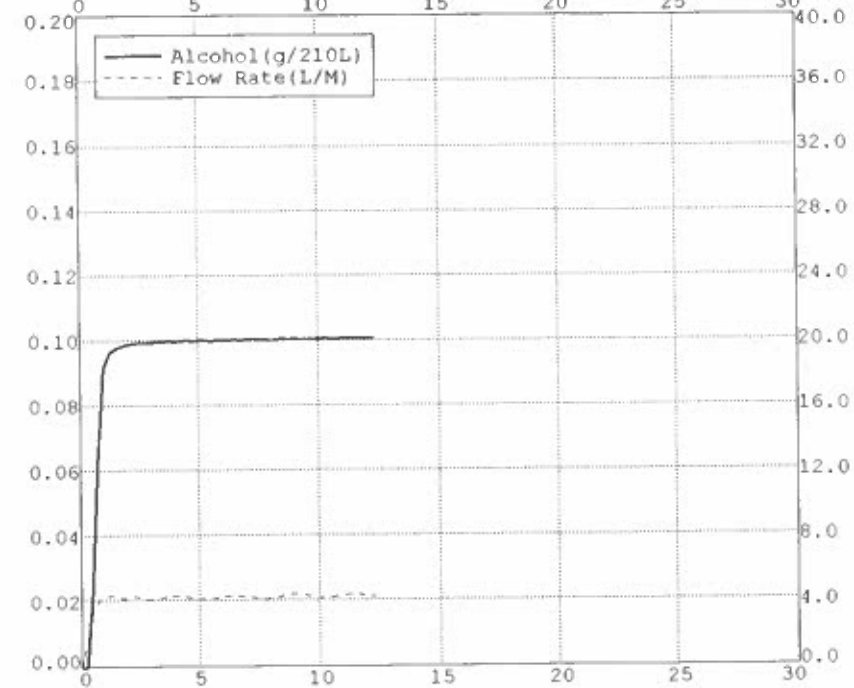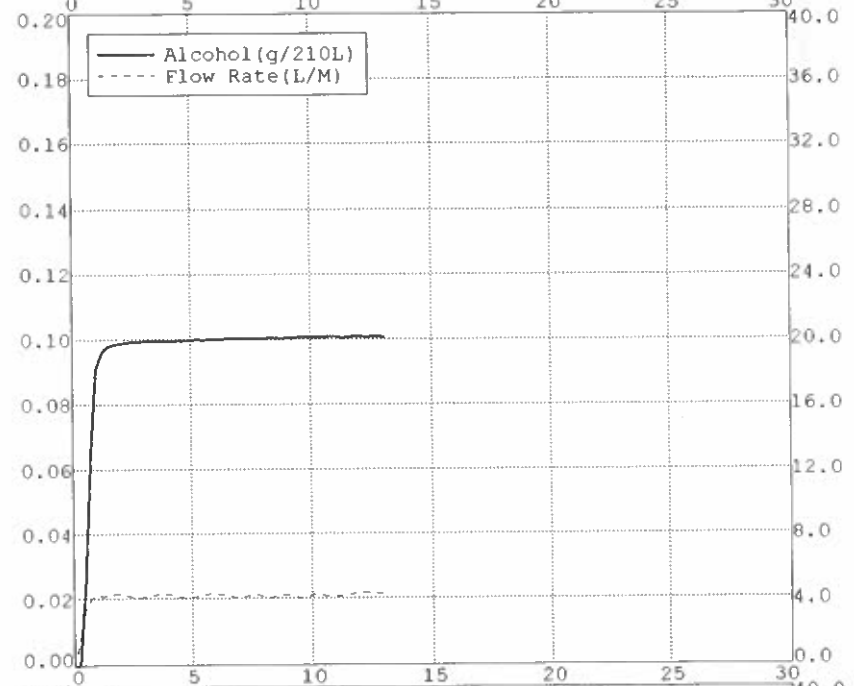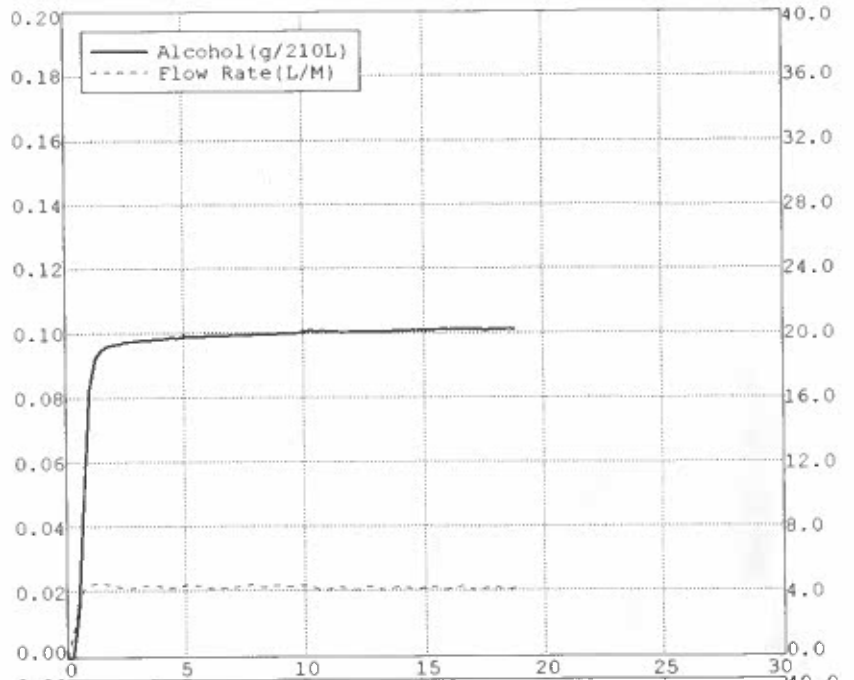

SOLUTION CHANGE

AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 02/01/2022

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:57
INTERNAL STANDARD	VERIFIED	12:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:57
BLANK TEST	0.00	12:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:58
BLANK TEST	0.00	12:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:00
BLANK TEST	0.00	13:00

