

SOLUTION CHANGE




AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 02/01/2024

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 23430

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:24
INTERNAL STANDARD	VERIFIED	08:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:25
BLANK TEST	0.00	08:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:26
BLANK TEST	0.00	08:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:27
BLANK TEST	0.00	08:28

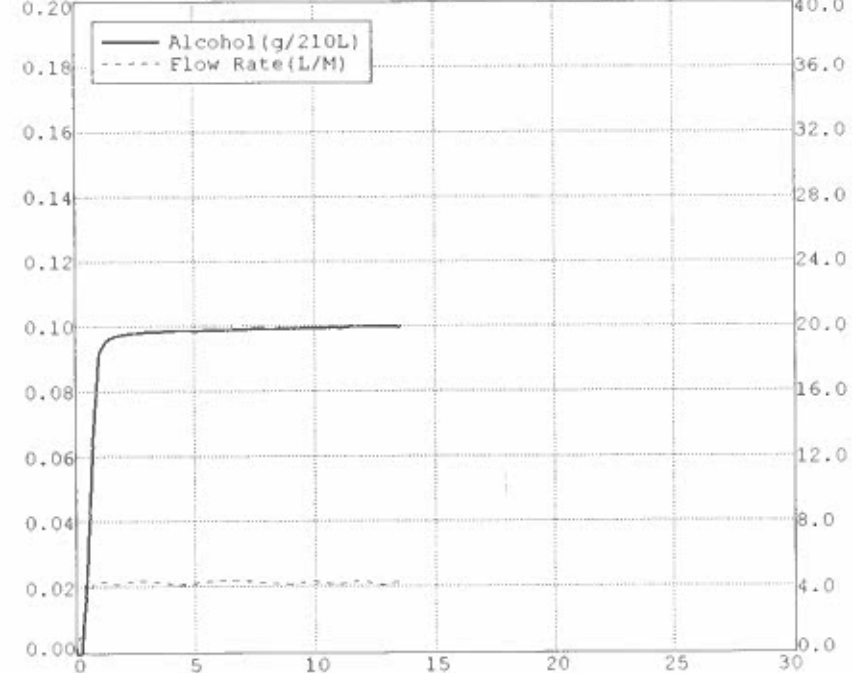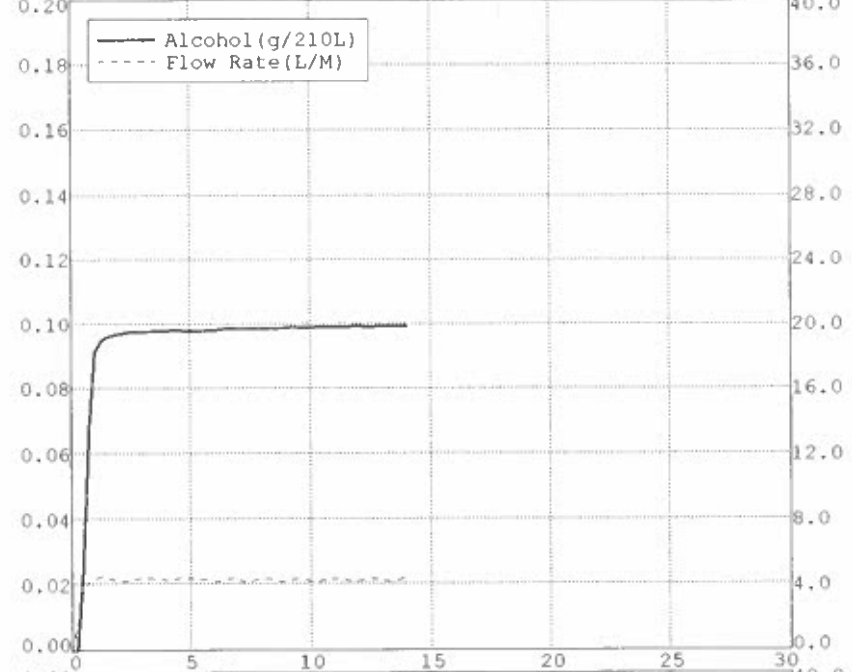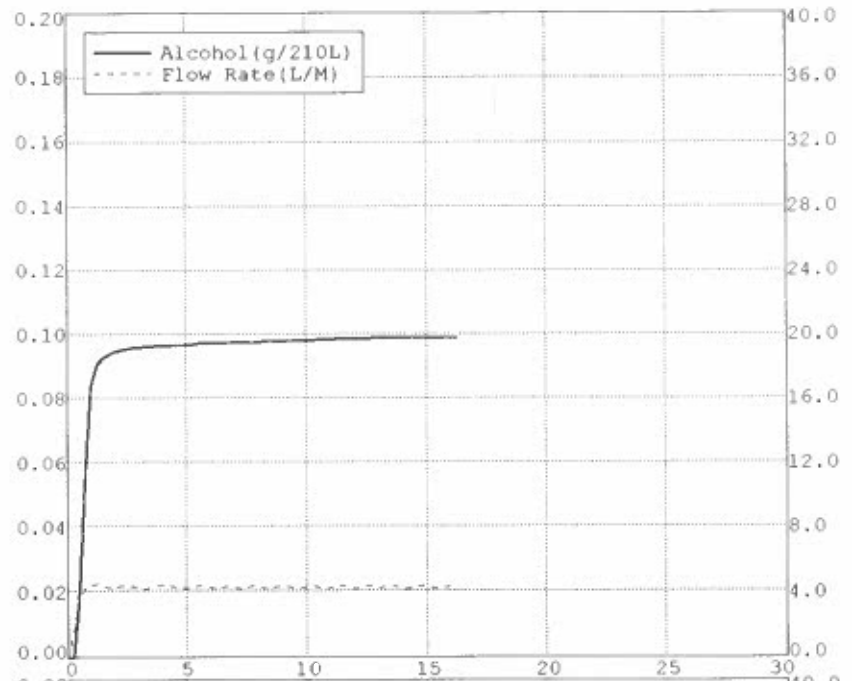

SUPERVISOR TEST

AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 02/01/2024

OPERATOR NAME:
 GREGORY D GILFUS *GD*
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:04
INTERNAL STANDARD	VERIFIED	08:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:04
BLANK TEST	0.00	08:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:05
BLANK TEST	0.00	08:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:06
BLANK TEST	0.00	08:07

