

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 02/03/2023

OPERATOR NAME: GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 22390

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:46
INTERNAL STANDARD	VERIFIED	07:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	07:47
BLANK TEST	0.00	07:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:48
BLANK TEST	0.00	07:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:49
BLANK TEST	0.00	07:50

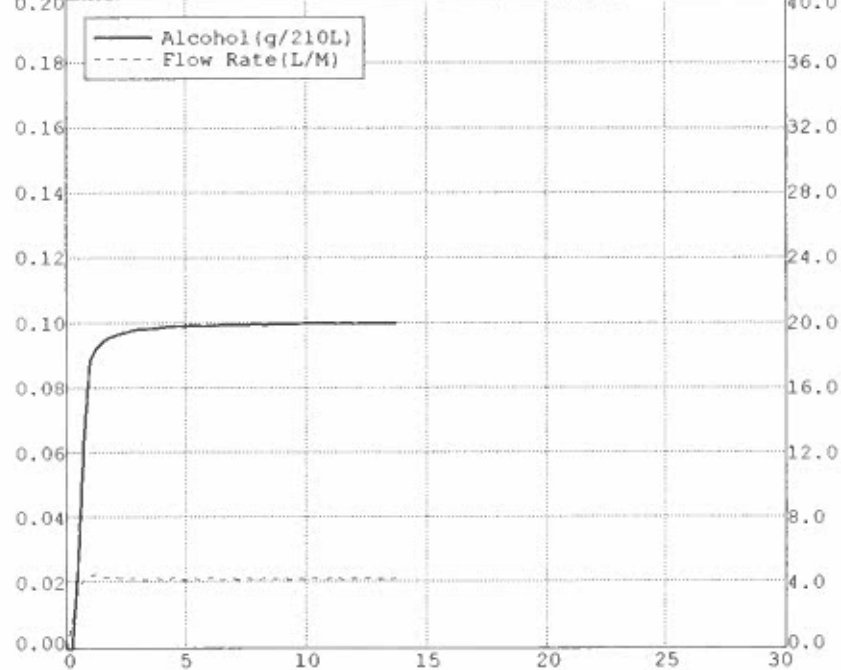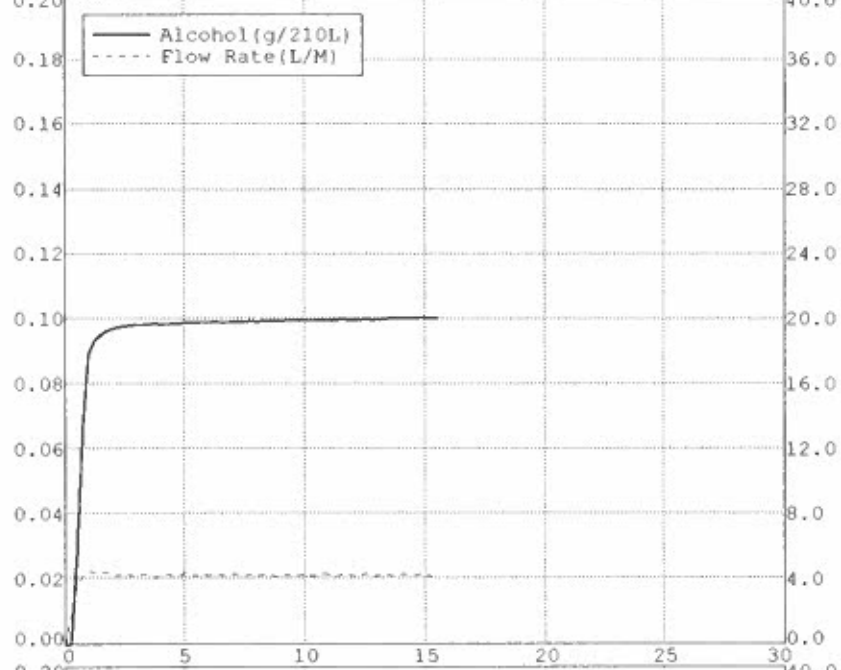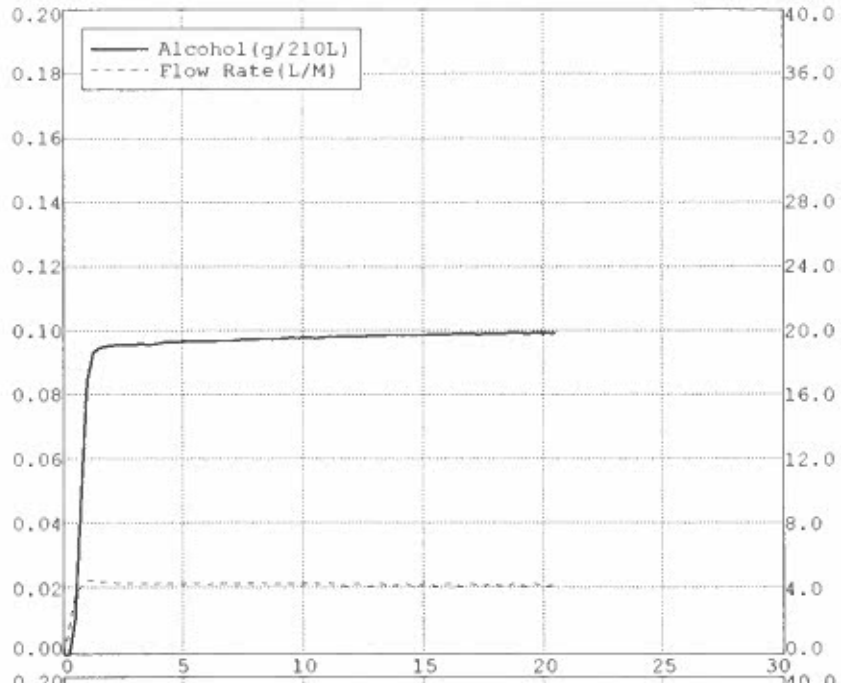

SOLUTION CHANGE

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 02/03/2023

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:01
INTERNAL STANDARD	VERIFIED	08:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:02
BLANK TEST	0.00	08:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	08:03
BLANK TEST	0.00	08:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	08:04
BLANK TEST	0.00	08:05

