

SOLUTION CHANGE




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 03/01/2021

OPERATOR NAME: *[Signature]*
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:53
INTERNAL STANDARD	VERIFIED	11:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:53
BLANK TEST	0.00	11:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:55
BLANK TEST	0.00	11:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:56
BLANK TEST	0.00	11:57

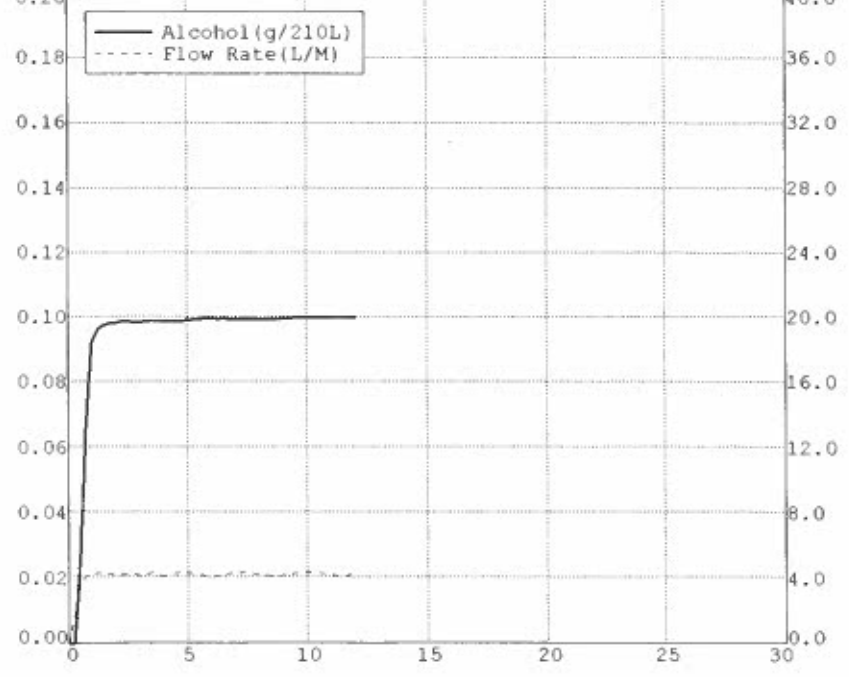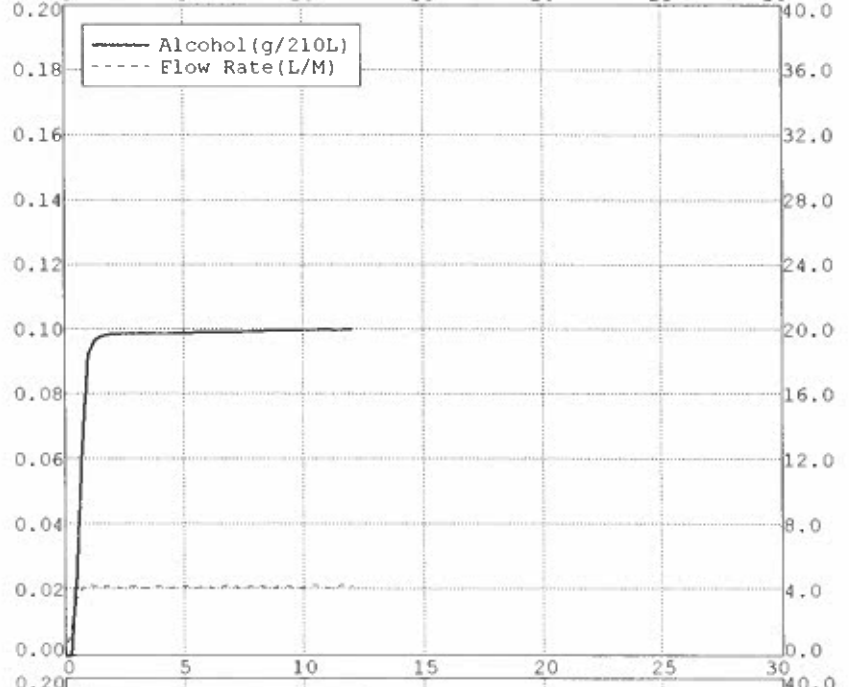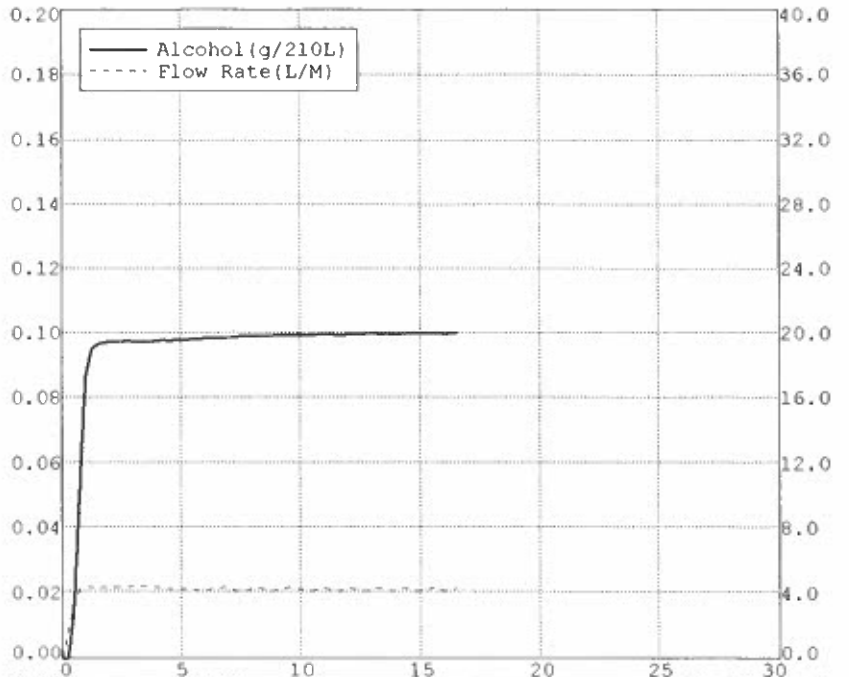

SUPERVISOR TEST

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 03/01/2021

OPERATOR NAME: GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:38
INTERNAL STANDARD	VERIFIED	08:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:39
BLANK TEST	0.00	08:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:40
BLANK TEST	0.00	08:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:41
BLANK TEST	0.00	08:42

