

SOLUTION CHANGE



 AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 04/01/2021

OPERATOR NAME: *[Signature]*
 GREGORY D GILFUE
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:30
INTERNAL STANDARD	VERIFIED	10:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:30
BLANK TEST	0.00	10:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:32
BLANK TEST	0.00	10:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:33
BLANK TEST	0.00	10:34

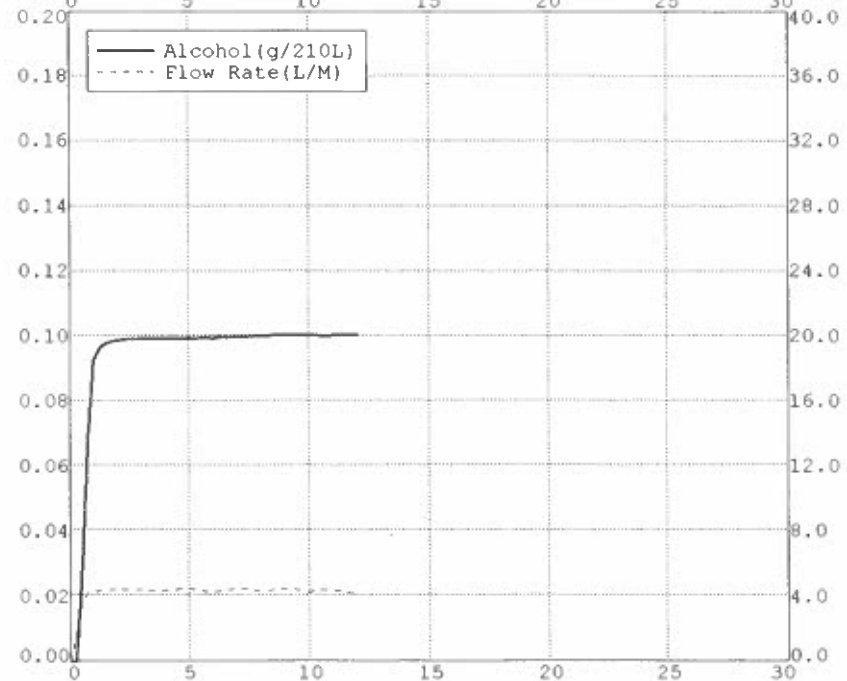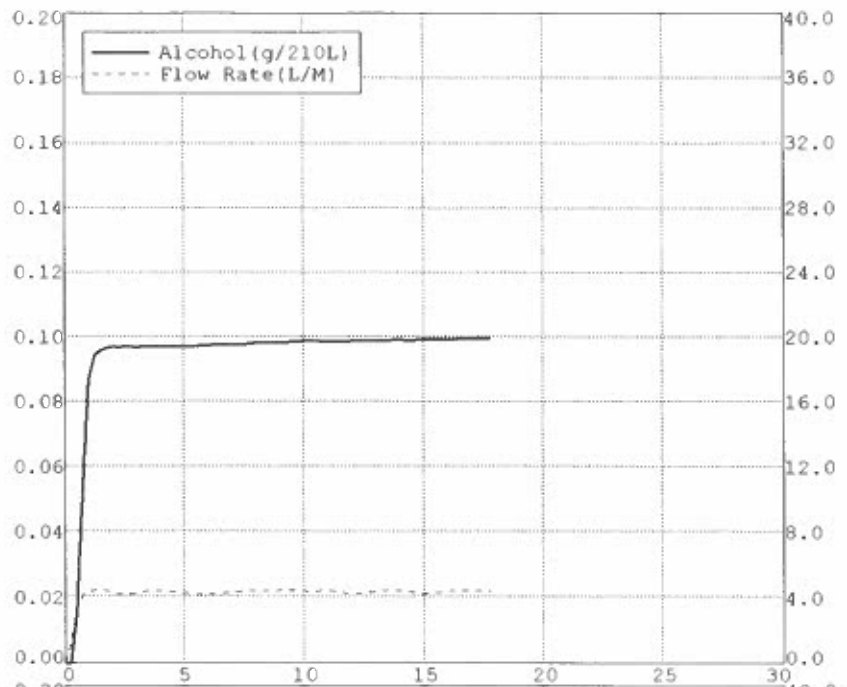

SUPERVISOR TEST

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 04/01/2021

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:59
INTERNAL STANDARD	VERIFIED	07:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:59
BLANK TEST	0.00	08:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:01
BLANK TEST	0.00	08:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:02
BLANK TEST	0.00	08:03

