

SOLUTION CHANGE




AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 04/01/2022

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:16
INTERNAL STANDARD	VERIFIED	08:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:17
BLANK TEST	0.00	08:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:18
BLANK TEST	0.00	08:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:19
BLANK TEST	0.00	08:20

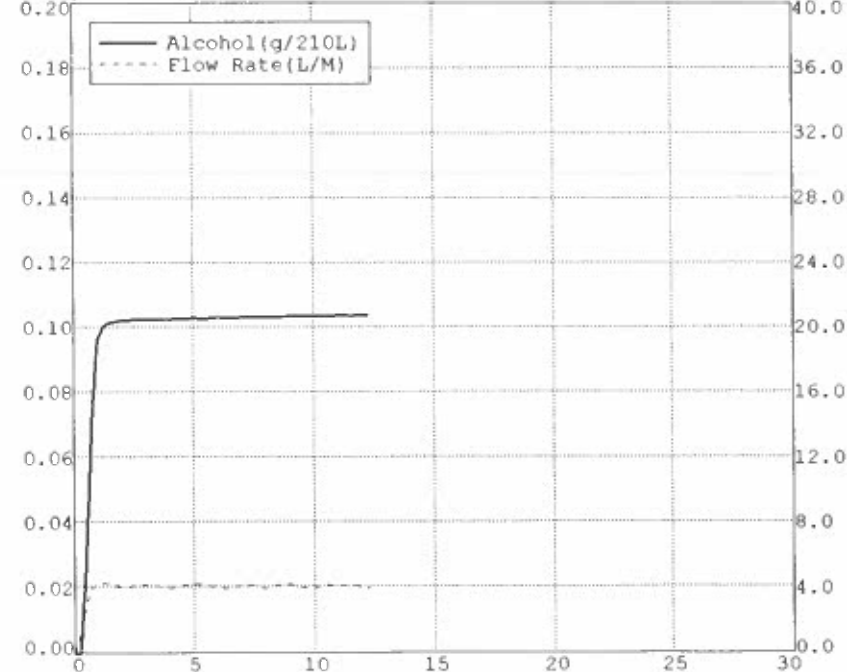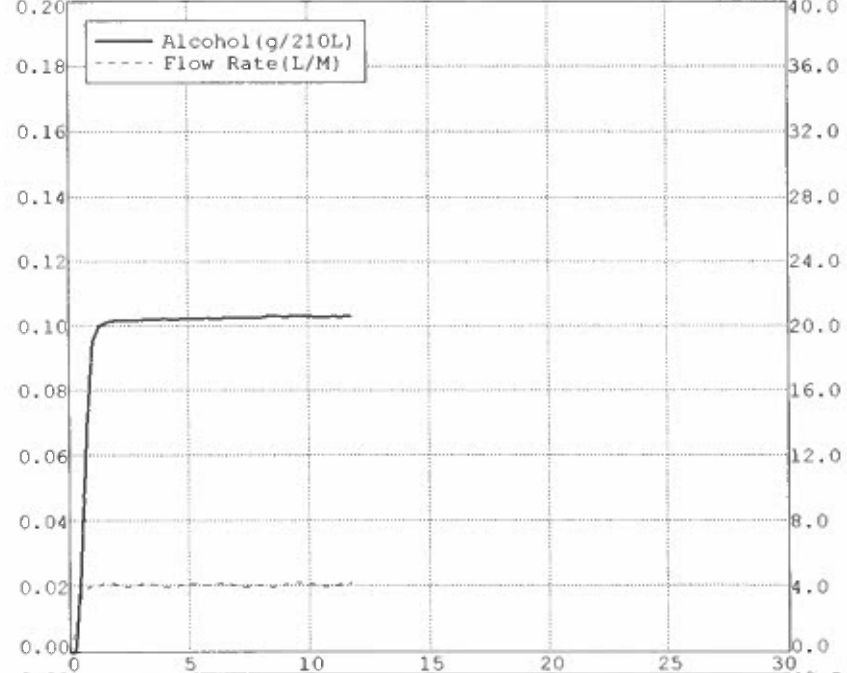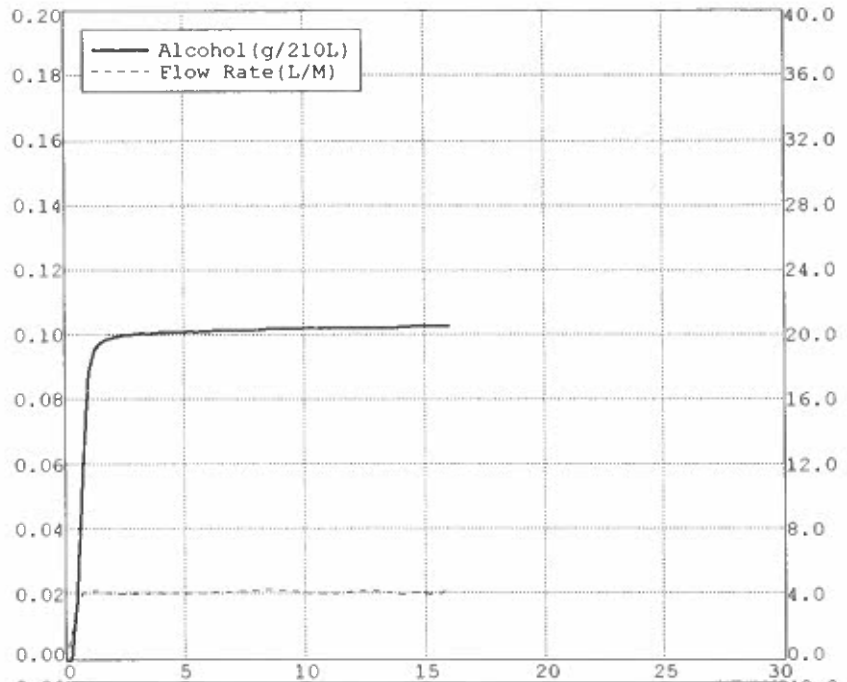

SUPERVISOR TEST

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 04/01/2022

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:51
INTERNAL STANDARD	VERIFIED	07:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:52
BLANK TEST	0.00	07:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:53
BLANK TEST	0.00	07:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:54
BLANK TEST	0.00	07:55

