

SOLUTION CHANGE




AUBURN CITY  
 POLICE DEPT  
 DATAMASTER dmt: 105406

Date: 04/02/2024

OPERATOR NAME:  
 GREGORY D GILFUS  
 Permit #: 30728  
 Operator Agency/Dept: AUBURN CITY PD  
 Reference Standard #: 24040

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:14
INTERNAL STANDARD	VERIFIED	14:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:15
BLANK TEST	0.00	14:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:16
BLANK TEST	0.00	14:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:17
BLANK TEST	0.00	14:18

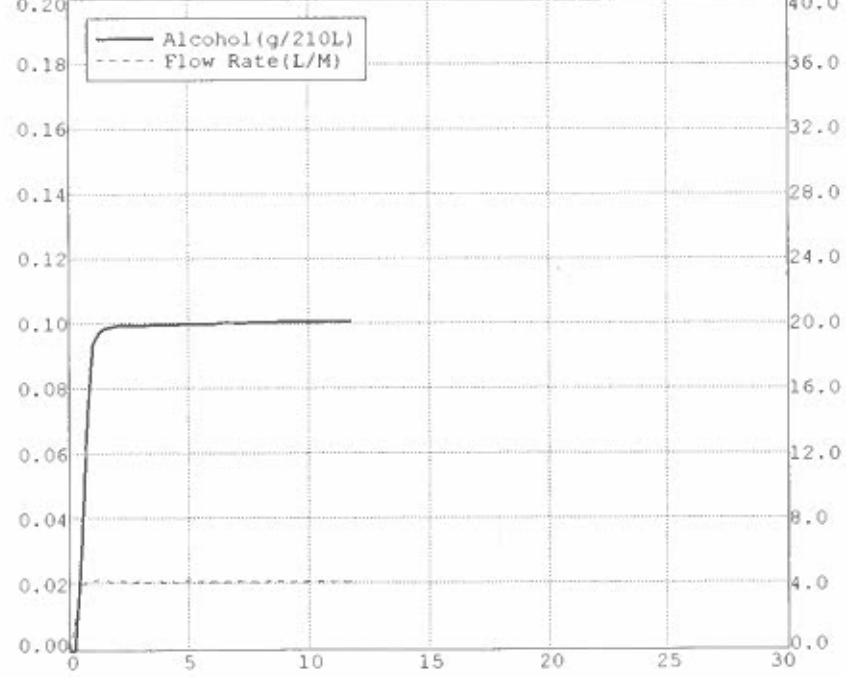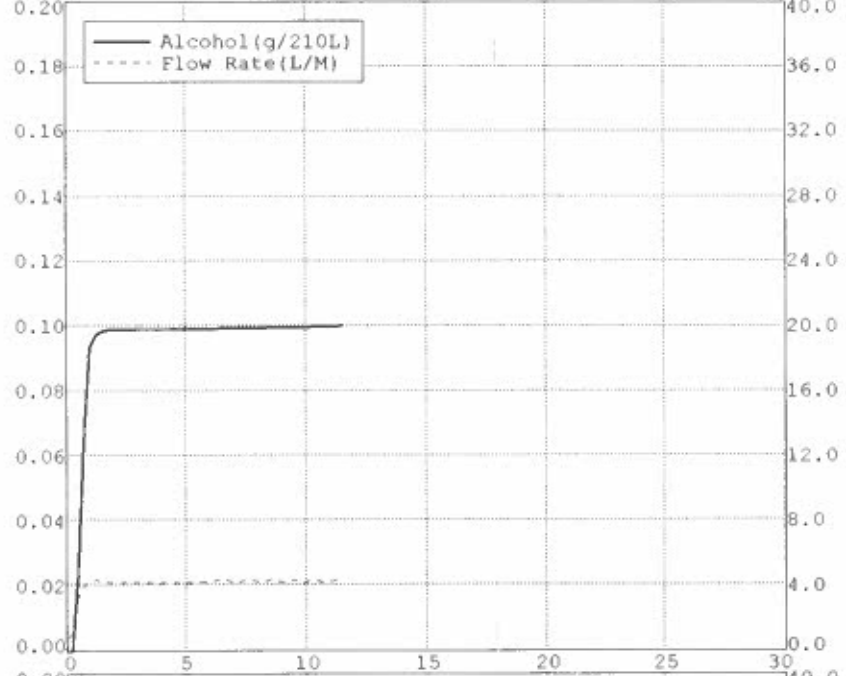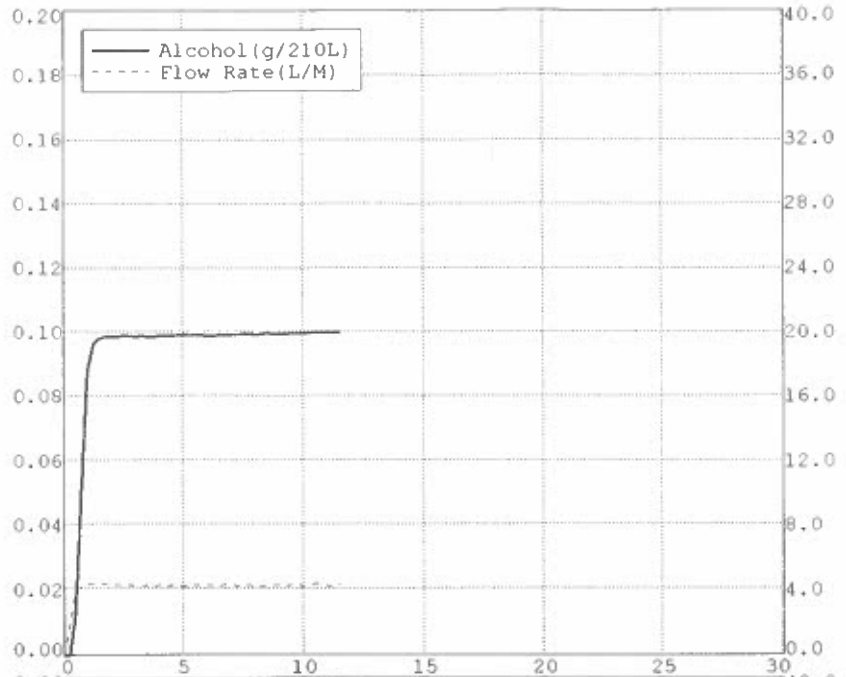

SUPERVISOR TEST

AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 04/02/2024

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 23430

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:14
INTERNAL STANDARD	VERIFIED	07:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:14
BLANK TEST	0.00	07:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:16
BLANK TEST	0.00	07:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:17
BLANK TEST	0.00	07:18

