

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 04/03/2023

OPERATOR NAME: GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 22420

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:29
INTERNAL STANDARD	VERIFIED	07:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	07:29
BLANK TEST	0.00	07:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:30
BLANK TEST	0.00	07:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:32
BLANK TEST	0.00	07:33

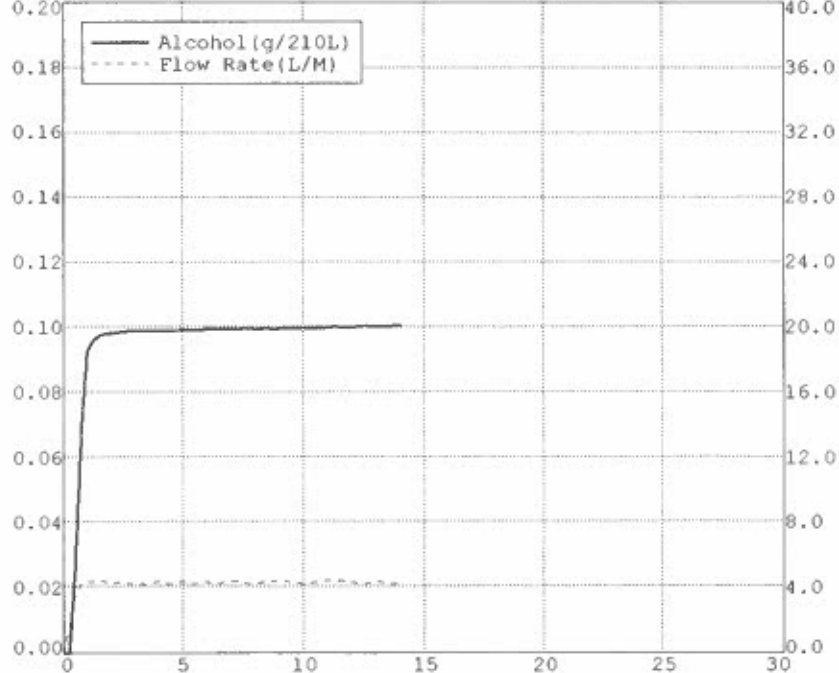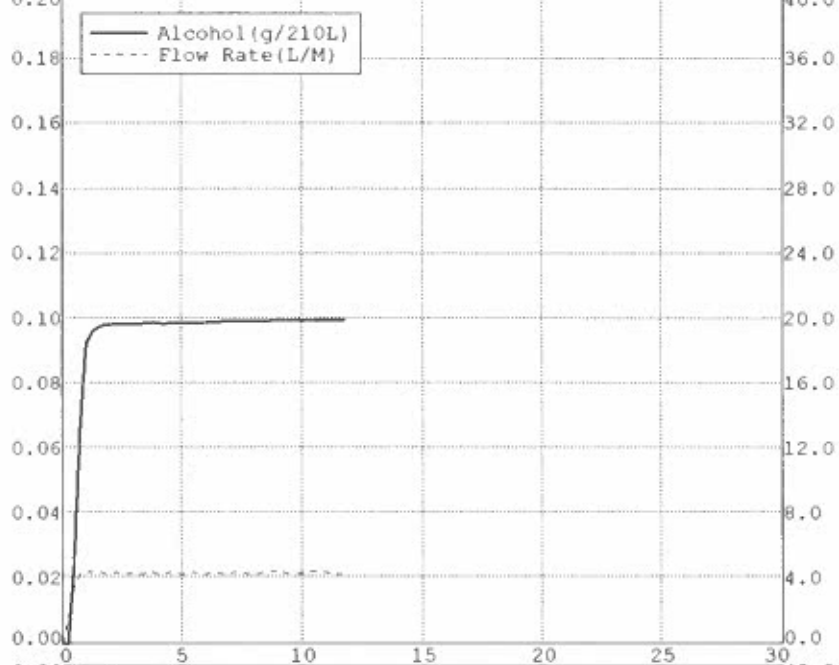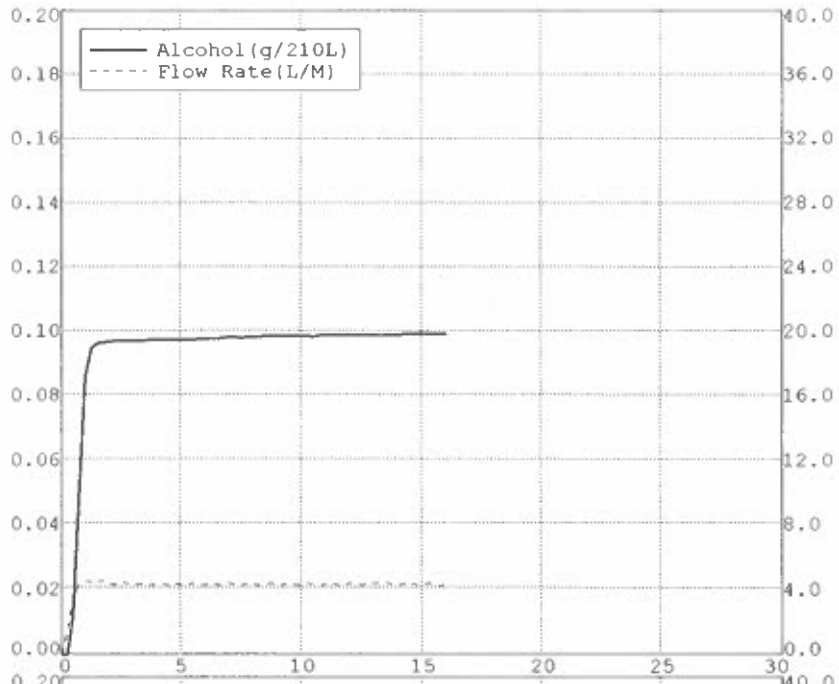

SOLUTION CHANGE

AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 04/03/2023

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:05
INTERNAL STANDARD	VERIFIED	08:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:05
BLANK TEST	0.00	08:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:06
BLANK TEST	0.00	08:07
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	08:08
BLANK TEST	0.00	08:08

