

SOLUTION CHANGE




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 05/01/2021

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30720
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:17
INTERNAL STANDARD	VERIFIED	09:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:17
BLANK TEST	0.00	09:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:19
BLANK TEST	0.00	09:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:20
BLANK TEST	0.00	09:21

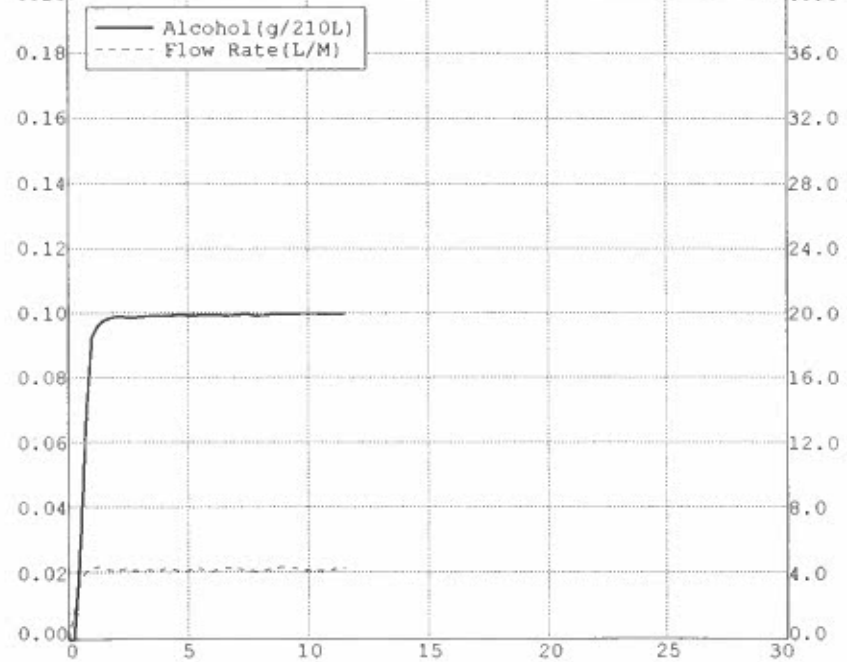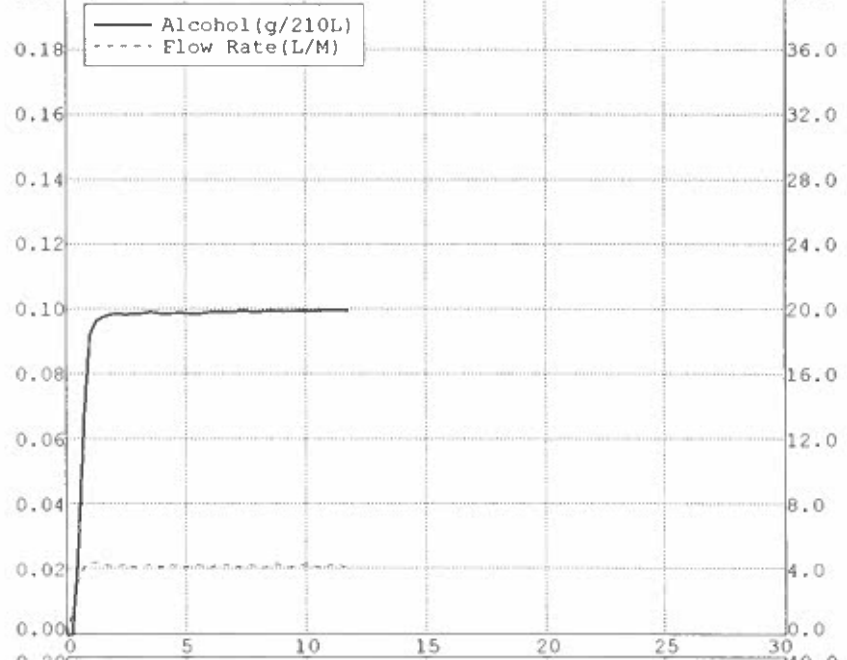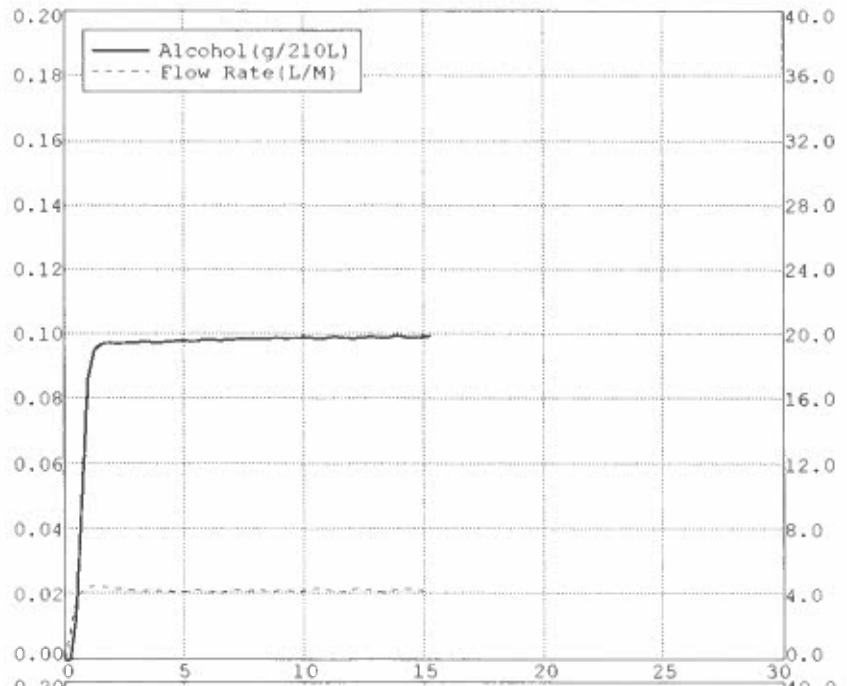

SUPERVISOR TEST

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 05/01/2021

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 21020
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:12
INTERNAL STANDARD	VERIFIED	07:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:12
BLANK TEST	0.00	07:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:14
BLANK TEST	0.00	07:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:15
BLANK TEST	0.00	07:16

