

SUPERVISOR TEST




AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 05/01/2024

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 24040

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:34
INTERNAL STANDARD	VERIFIED	07:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:34
BLANK TEST	0.00	07:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:36
BLANK TEST	0.00	07:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:37
BLANK TEST	0.00	07:38

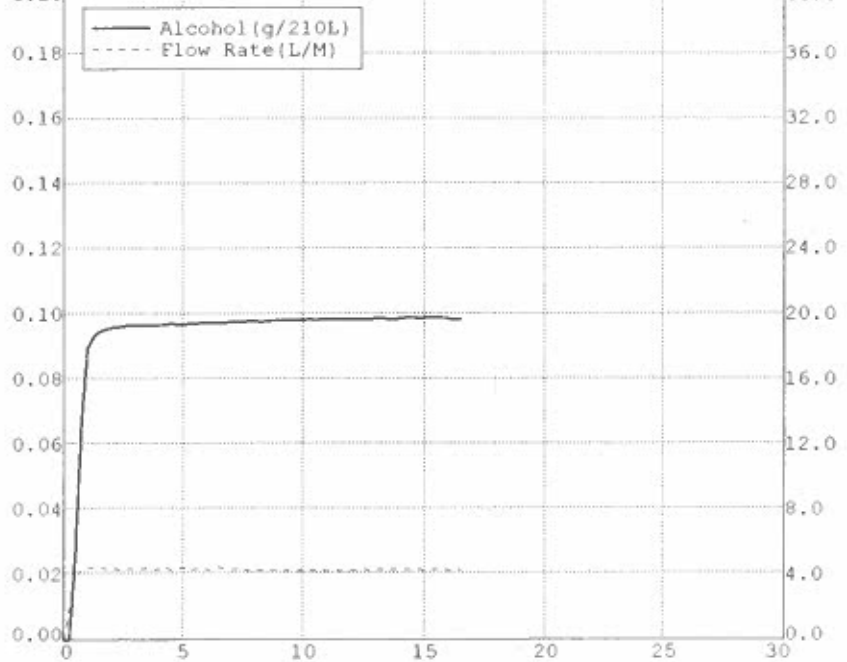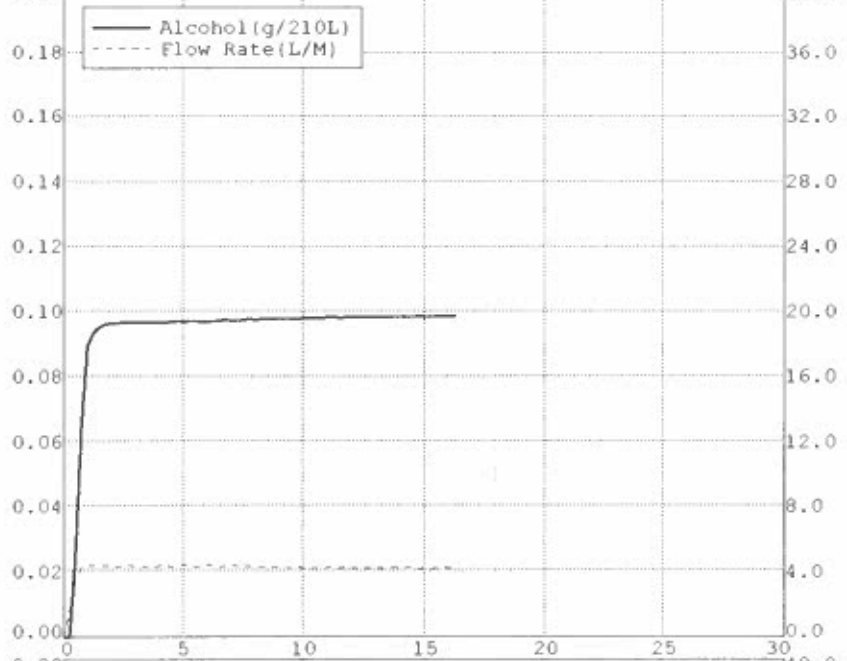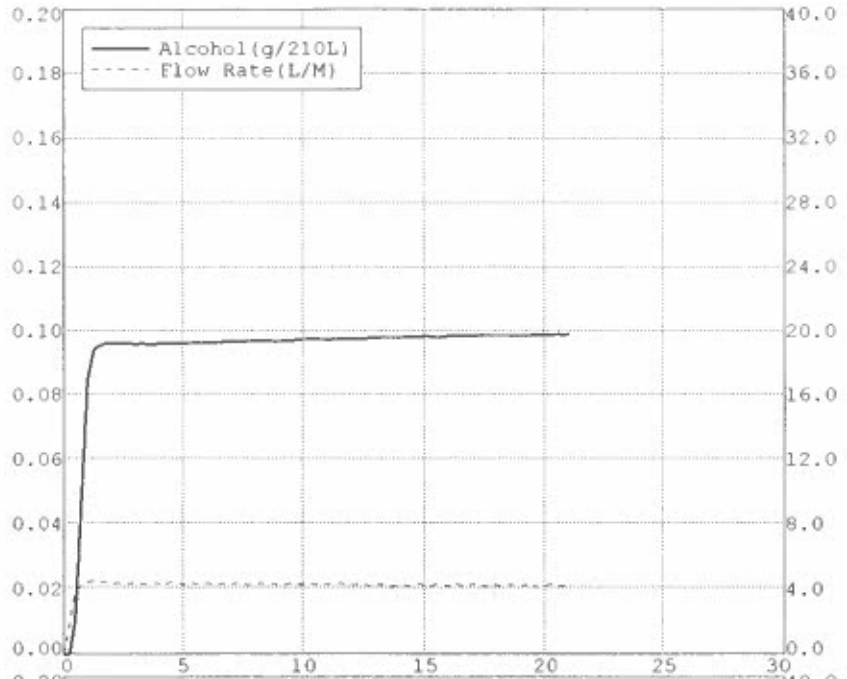

SOLUTION CHANGE

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 05/01/2024

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 24040

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:07
INTERNAL STANDARD	VERIFIED	08:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:08
BLANK TEST	0.00	08:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:09
BLANK TEST	0.00	08:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:10
BLANK TEST	0.00	08:11

