

SUPERVISOR TEST




AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 05/02/2022

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:14
INTERNAL STANDARD	VERIFIED	07:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:14
BLANK TEST	0.00	07:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:15
BLANK TEST	0.00	07:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:16
BLANK TEST	0.00	07:17

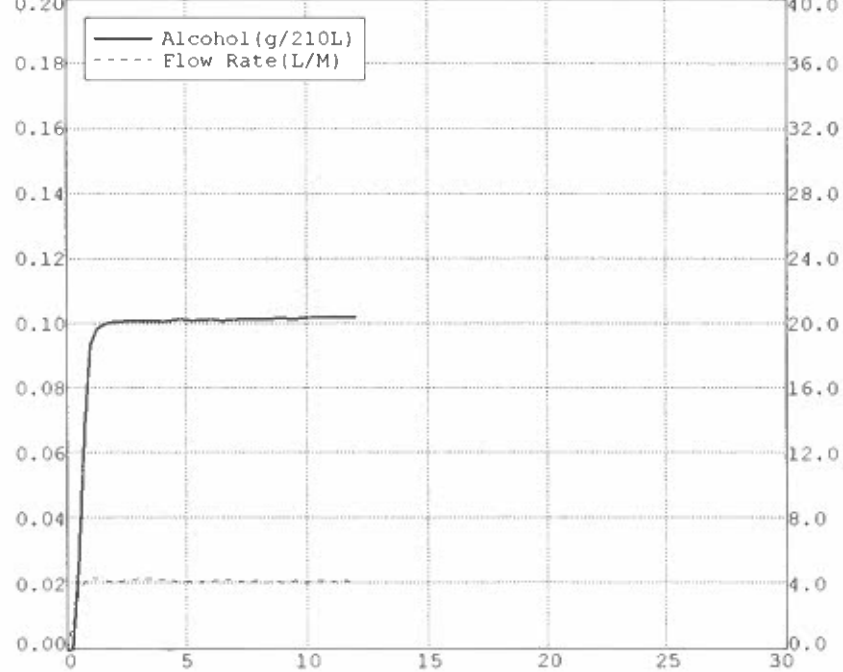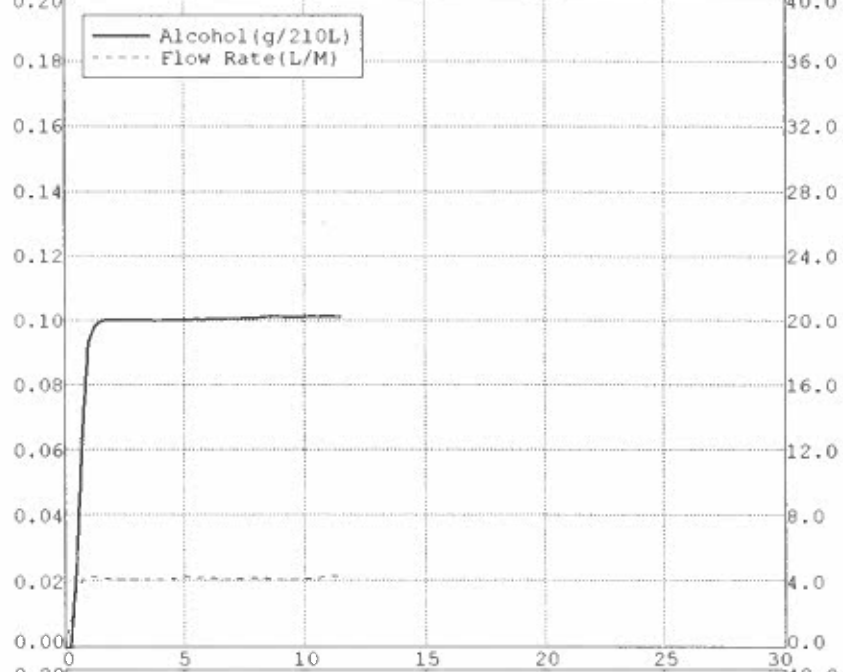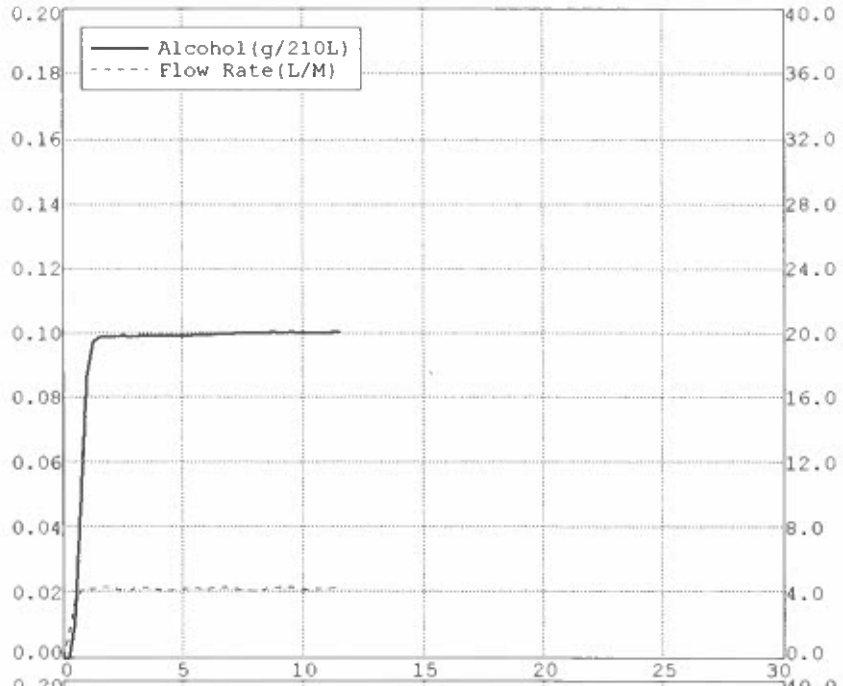

SOLUTION CHANGE

AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 05/02/2022

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:02
INTERNAL STANDARD	VERIFIED	08:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:02
BLANK TEST	0.00	08:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:03
BLANK TEST	0.00	08:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:05
BLANK TEST	0.00	08:05

