

SOLUTION CHANGE




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 06/01/2022

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:10
INTERNAL STANDARD	VERIFIED	10:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:10
BLANK TEST	0.00	10:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:11
BLANK TEST	0.00	10:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:13
BLANK TEST	0.00	10:14

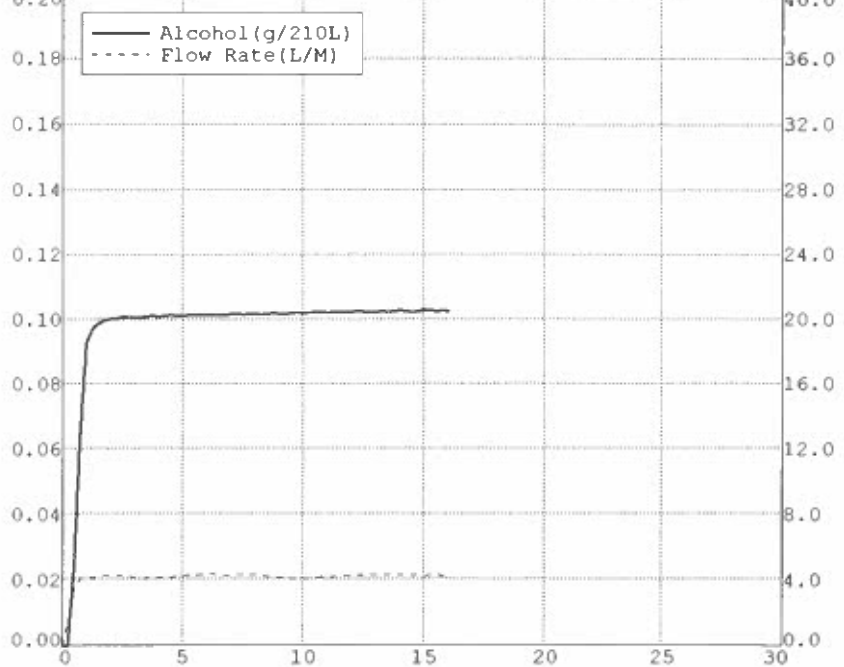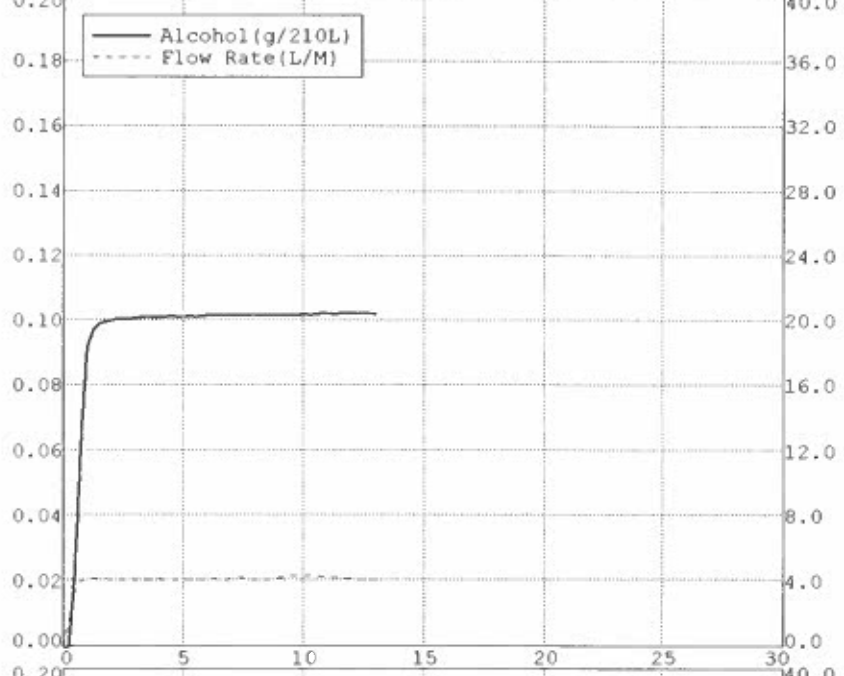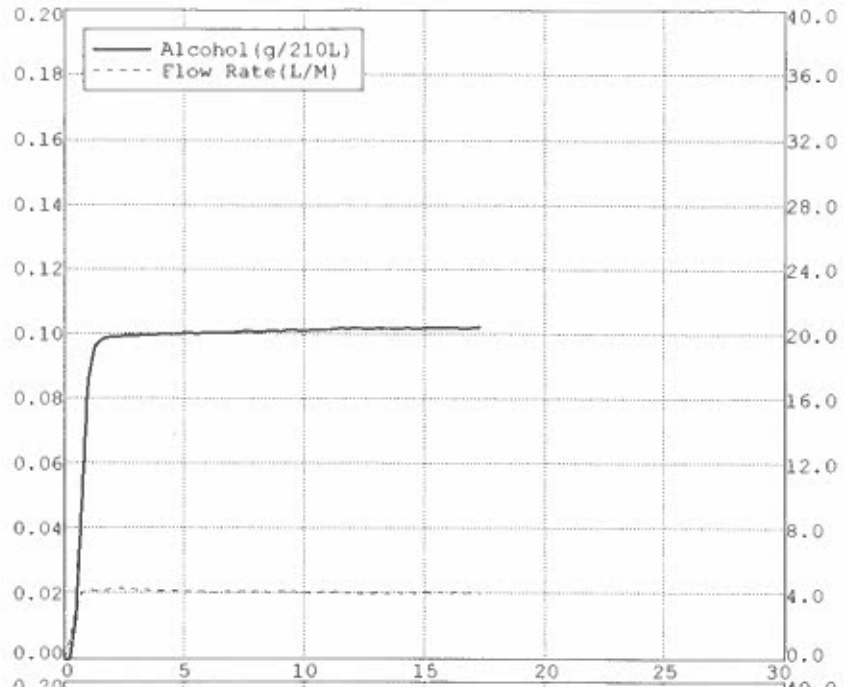

SUPERVISOR TEST

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 06/01/2022

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:50
INTERNAL STANDARD	VERIFIED	07:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:50
BLANK TEST	0.00	07:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:51
BLANK TEST	0.00	07:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:53
BLANK TEST	0.00	07:53

