

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 06/01/2023

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:45
INTERNAL STANDARD	VERIFIED	09:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:45
BLANK TEST	0.00	09:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:47
BLANK TEST	0.00	09:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:48
BLANK TEST	0.00	09:49

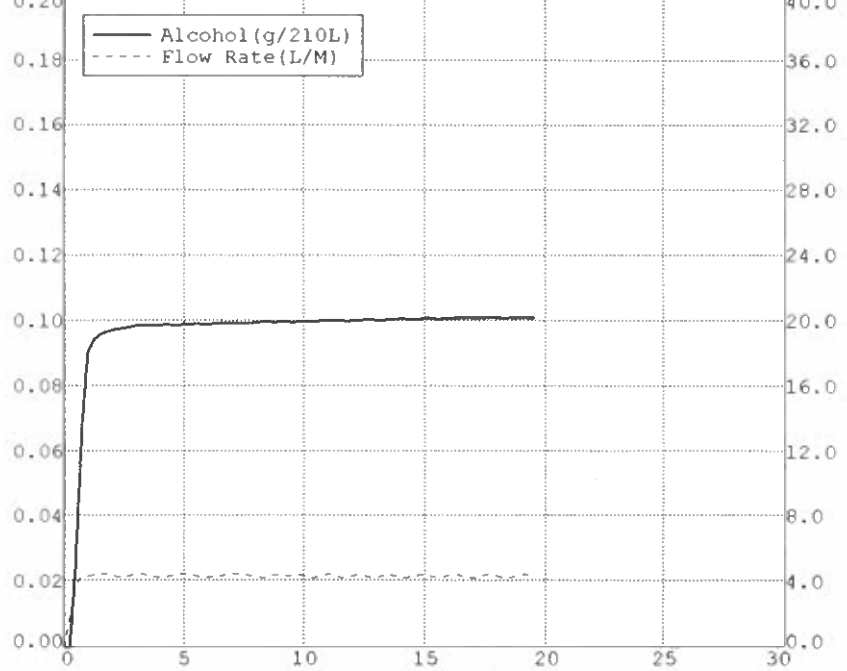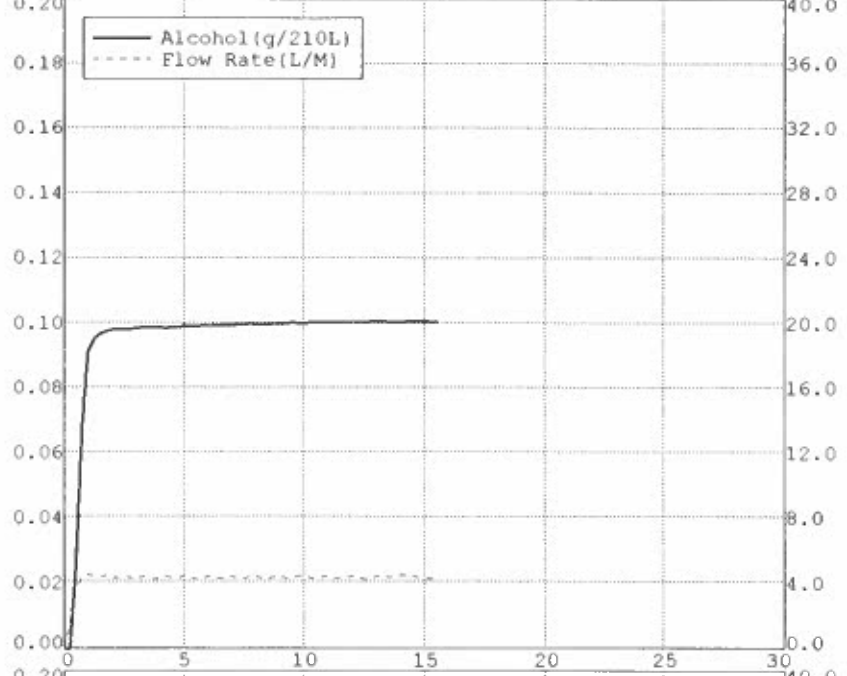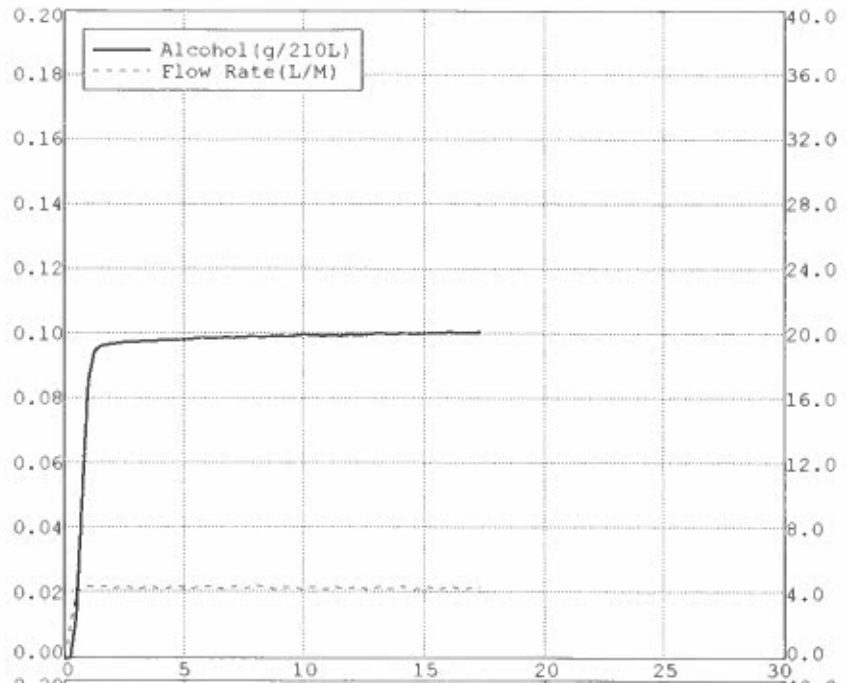

SOLUTION CHANGE

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 06/01/2023

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:59
INTERNAL STANDARD	VERIFIED	09:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	10:00
BLANK TEST	0.00	10:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:01
BLANK TEST	0.00	10:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:02
BLANK TEST	0.00	10:03

