

SOLUTION CHANGE




AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 07/03/2023

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:19
INTERNAL STANDARD	VERIFIED	09:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:19
BLANK TEST	0.00	09:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:20
BLANK TEST	0.00	09:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:22
BLANK TEST	0.00	09:23

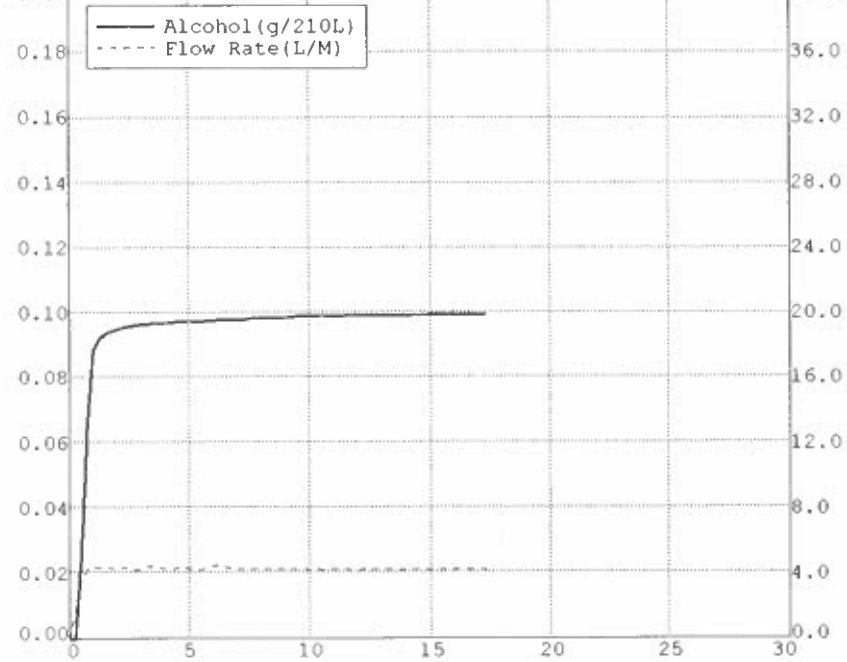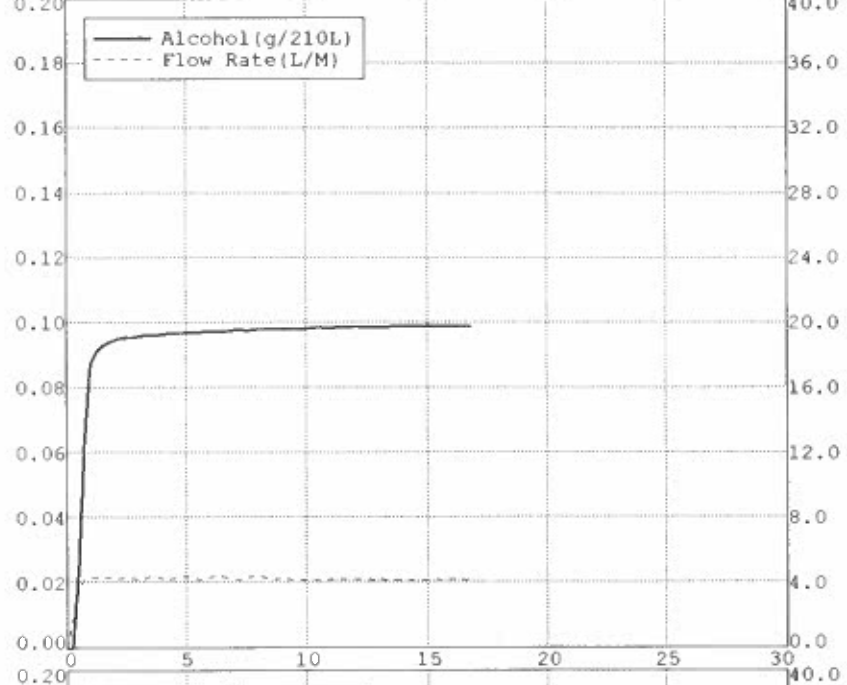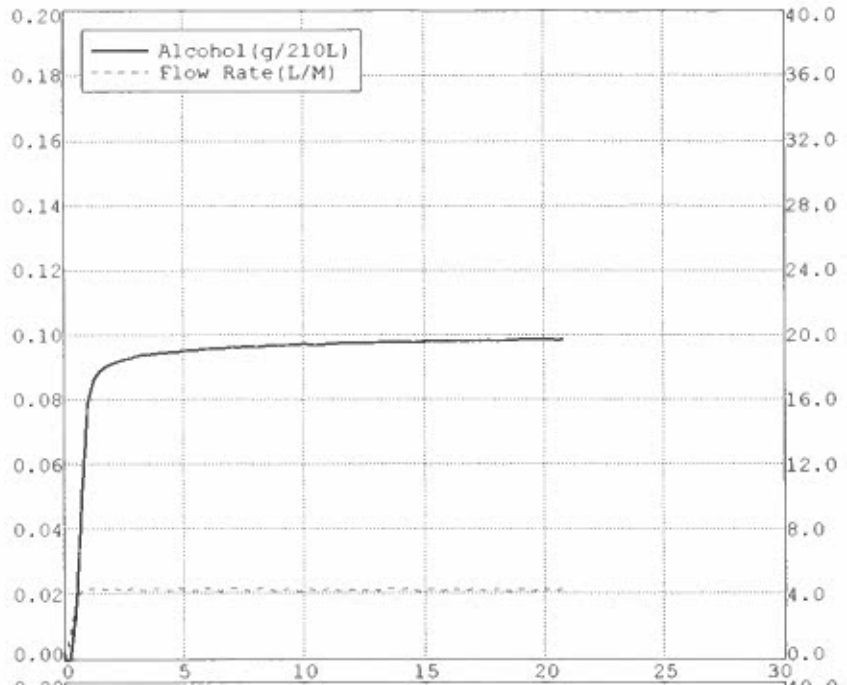

SUPERVISOR TEST

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 07/03/2023

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:03
INTERNAL STANDARD	VERIFIED	08:03
REFERENCE STANDARD TEMP	34.00e	
REFERENCE STANDARD	0.09	08:03
BLANK TEST	0.00	08:04
REFERENCE STANDARD TEMP	34.00e	
REFERENCE STANDARD	0.09	08:04
BLANK TEST	0.00	08:05
REFERENCE STANDARD TEMP	34.00e	
REFERENCE STANDARD	0.09	08:06
BLANK TEST	0.00	08:07

