

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 07/19/2022

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30726
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:49
INTERNAL STANDARD	VERIFIED	09:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:50
BLANK TEST	0.00	09:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:51
BLANK TEST	0.00	09:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:53
BLANK TEST	0.00	09:53

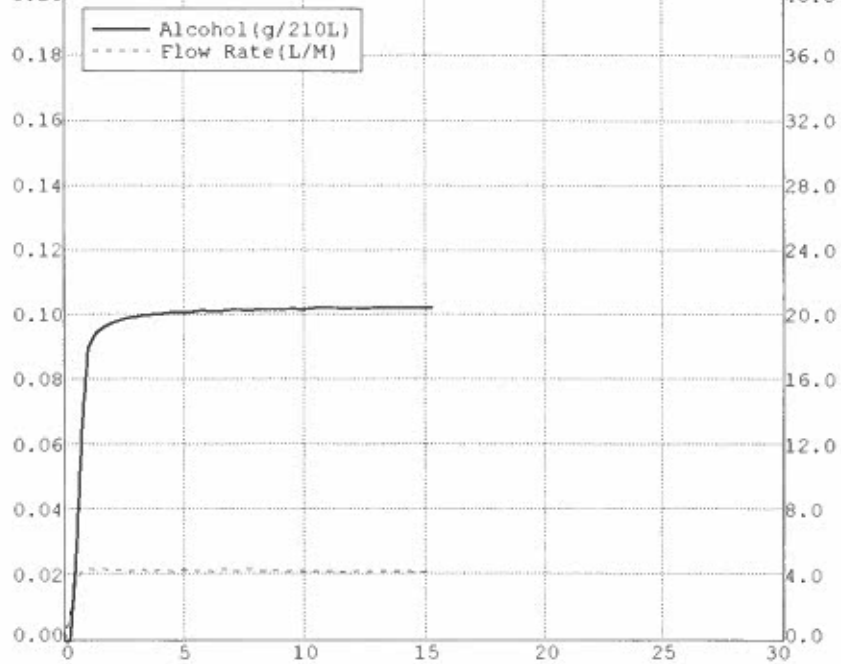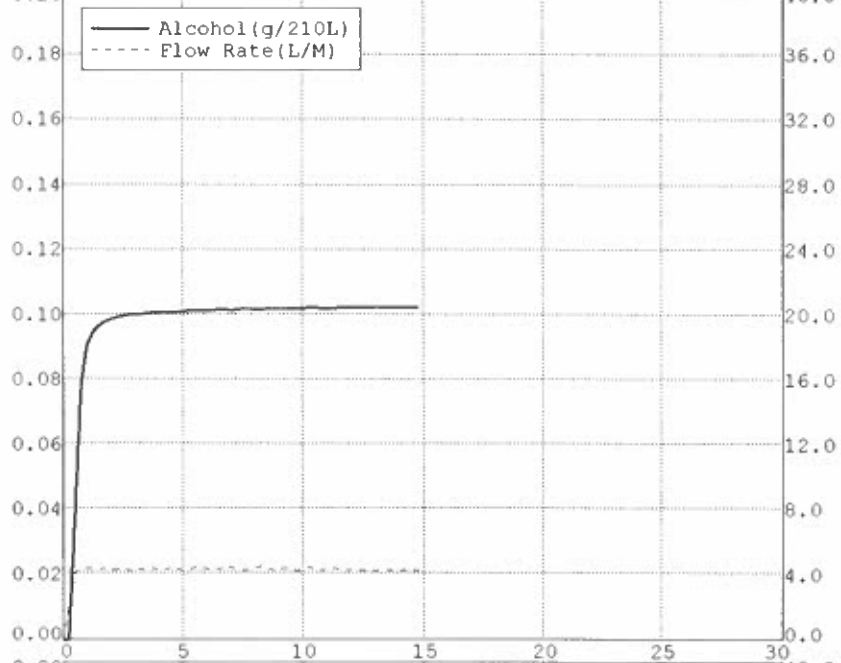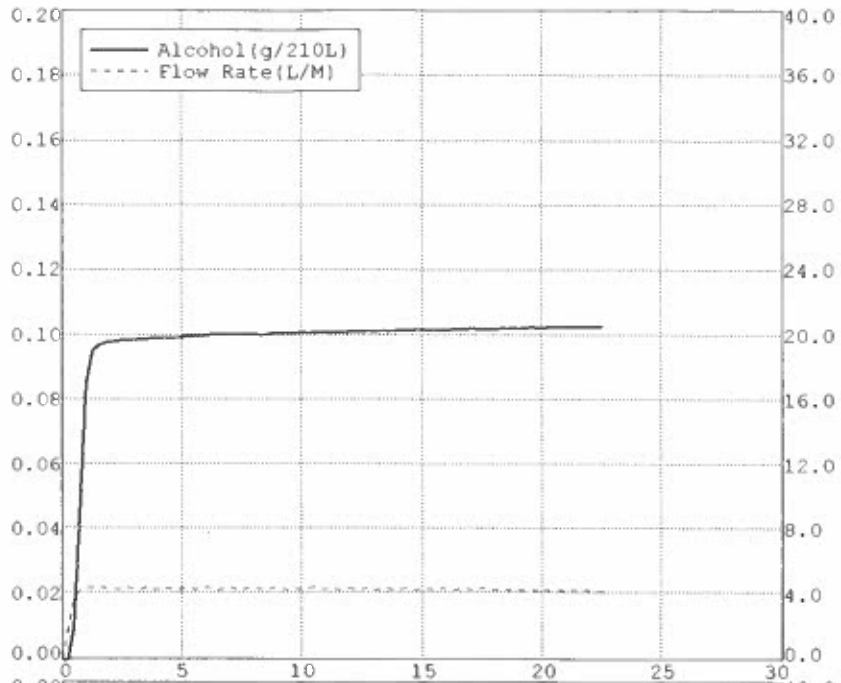

SOLUTION CHANGE

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 07/19/2022

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:14
INTERNAL STANDARD	VERIFIED	12:14
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:14
BLANK TEST	0.00	12:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:16
BLANK TEST	0.10	12:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:17
BLANK TEST	0.00	12:18

