

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 08/01/2022

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:09
INTERNAL STANDARD	VERIFIED	07:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	07:09
BLANK TEST	0.00	07:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:10
BLANK TEST	0.00	07:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:12
BLANK TEST	0.00	07:13

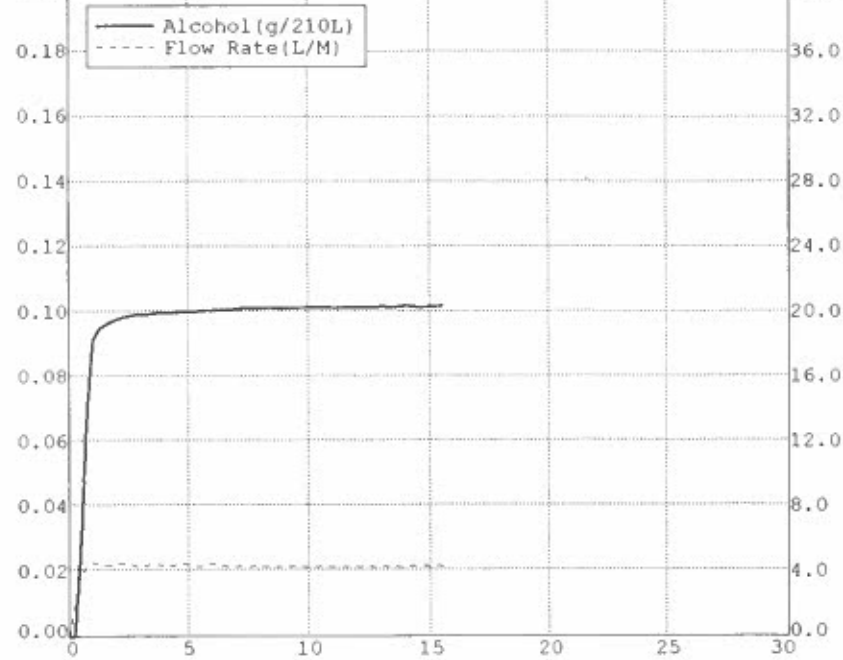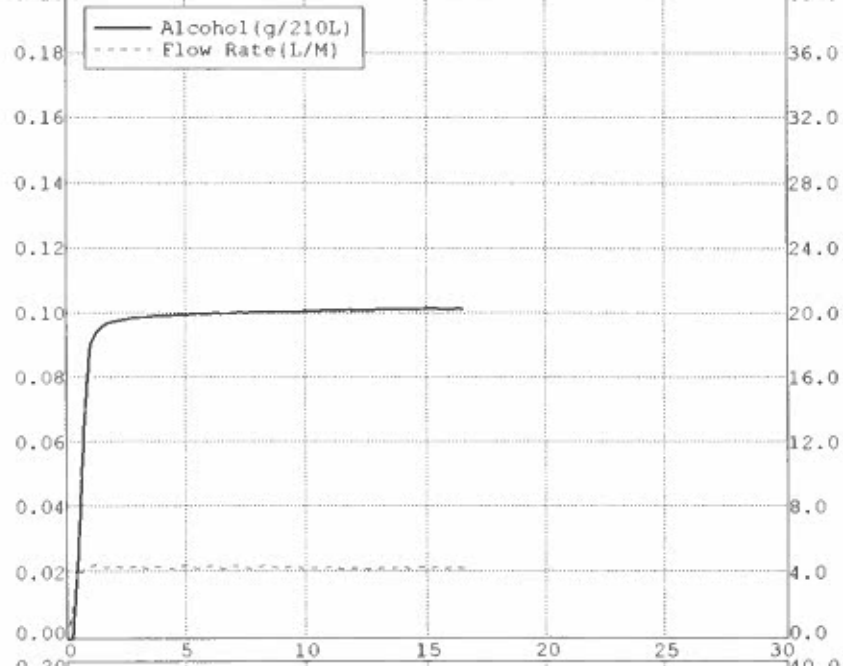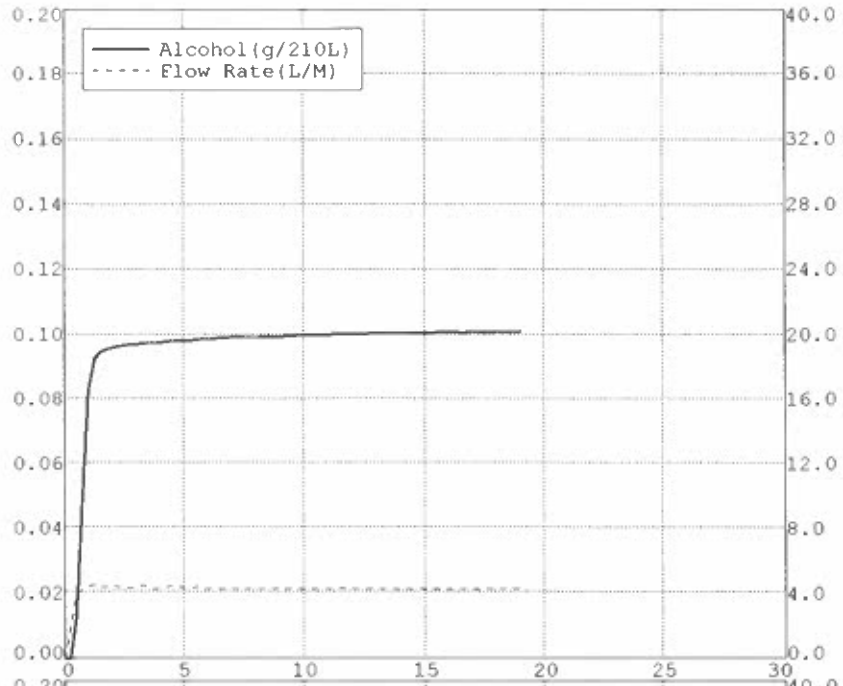

SOLUTION CHANGE

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 08/01/2022

OPERATOR NAME: GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:39
INTERNAL STANDARD	VERIFIED	07:40
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	07:40
BLANK TEST	0.00	07:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:41
BLANK TEST	0.00	07:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:43
BLANK TEST	0.00	07:43

