

SOLUTION CHANGE




AUBURN CITY  
 POLICE DEPT  
 DATAMASTER dmt: 105406

Date: 09/05/2023

OPERATOR NAME:  
 GREGORY D GILFUS  
 Permit #: 30728  
 Operator Agency/Dept: AUBURN CITY PD  
 Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:08
INTERNAL STANDARD	VERIFIED	09:08
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:09
BLANK TEST	0.00	09:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:10
BLANK TEST	0.00	09:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:11
BLANK TEST	0.00	09:12

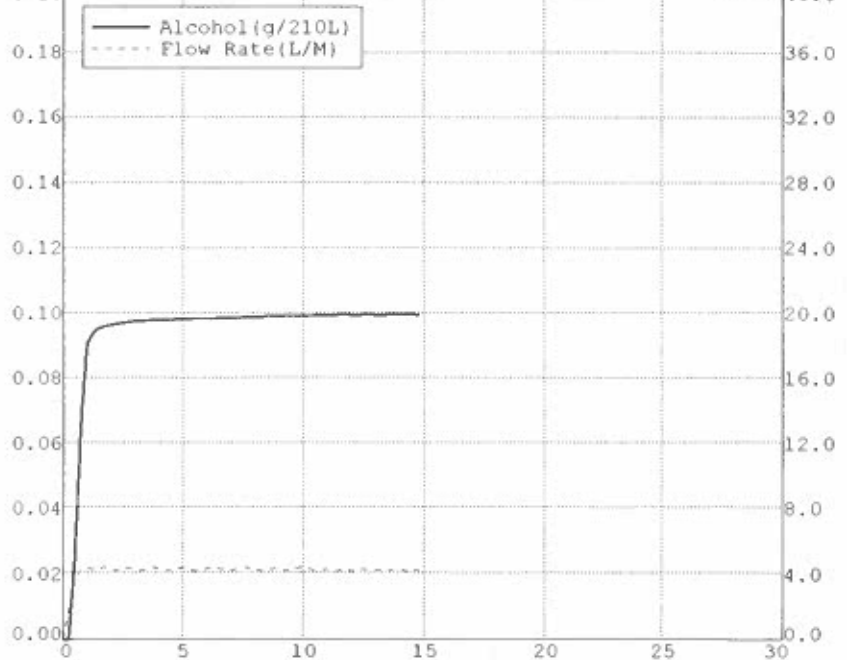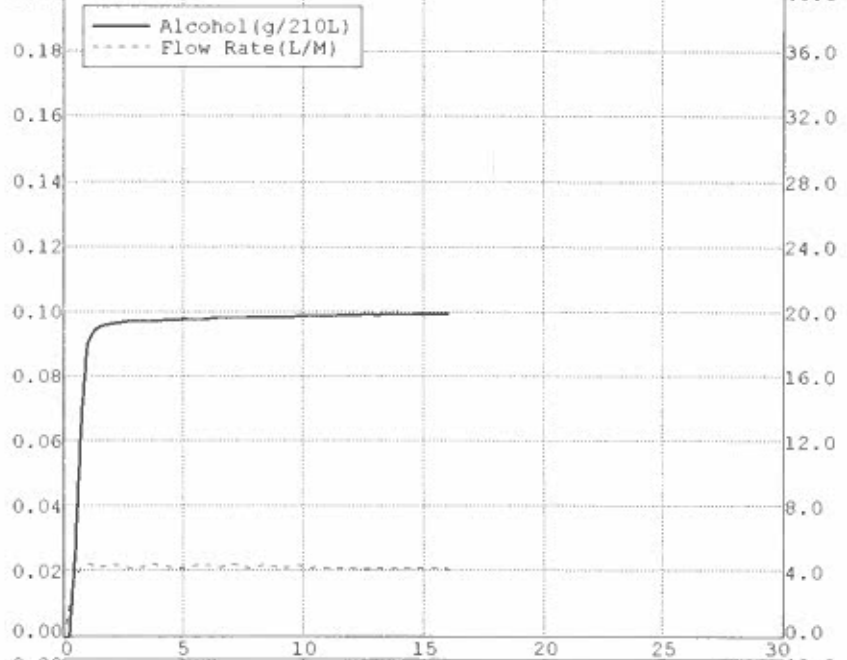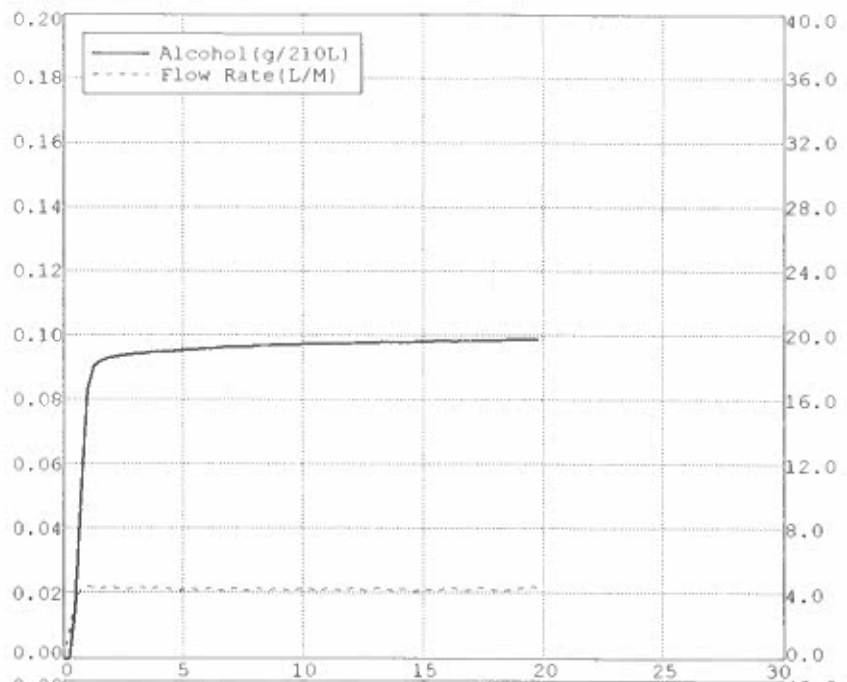

SUPERVISOR TEST

AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 09/05/2023

OPERATOR NAME: GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:26
INTERNAL STANDARD	VERIFIED	07:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:27
BLANK TEST	0.00	07:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:28
BLANK TEST	0.00	07:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:29
BLANK TEST	0.00	07:30

