

SOLUTION CHANGE




-----  
 AUBURN CITY  
 POLICE DEPT  
 DATAMASTER dmt: 105406  
 -----

Date: 10/01/2020

OPERATOR NAME:  
 GREGORY D GILFUS  
 Permit #: 30726  
 Operator Agency/Dept: AUBURN CITY PD  
 Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:26
INTERNAL STANDARD	VERIFIED	08:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:26
BLANK TEST	0.00	08:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:27
BLANK TEST	0.00	08:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:29
BLANK TEST	0.00	08:30

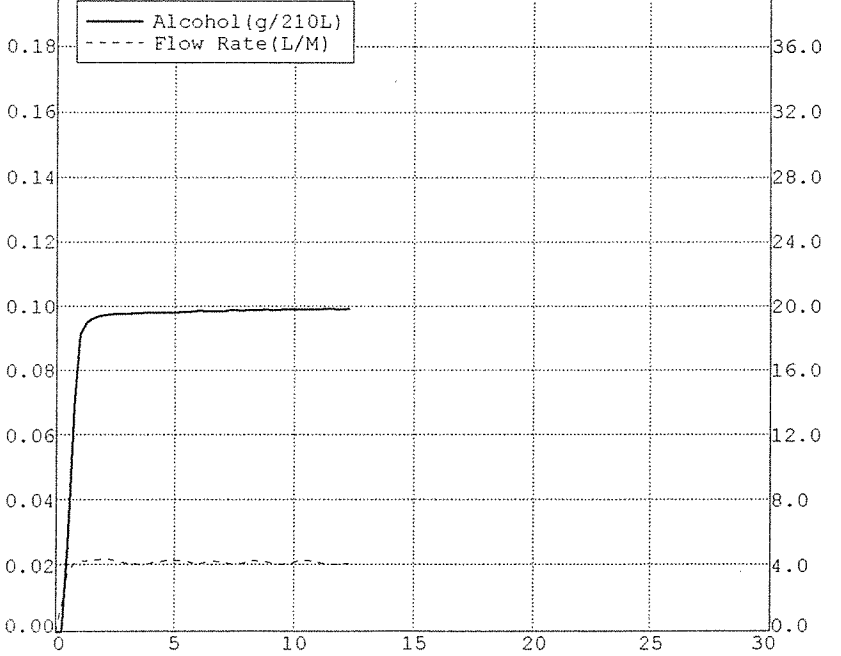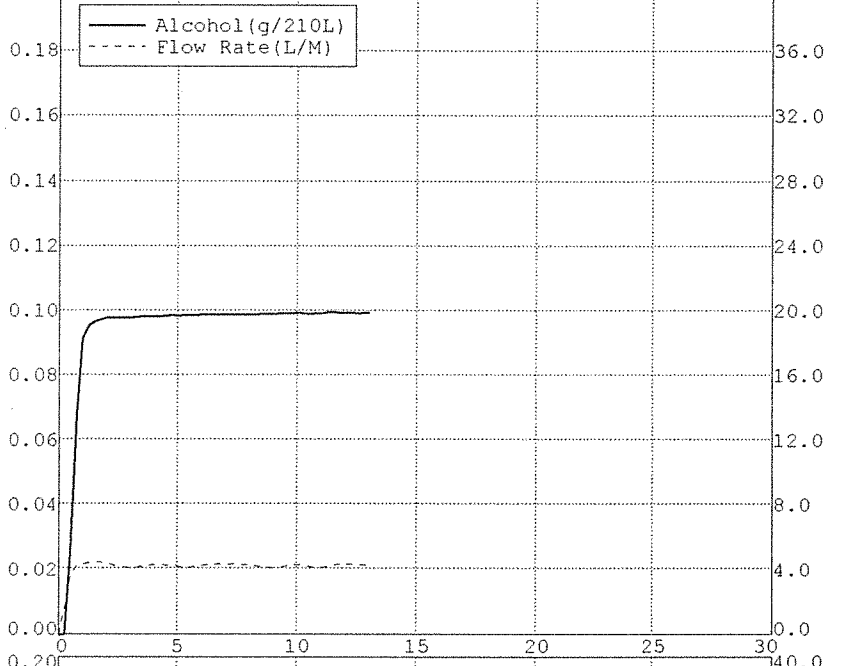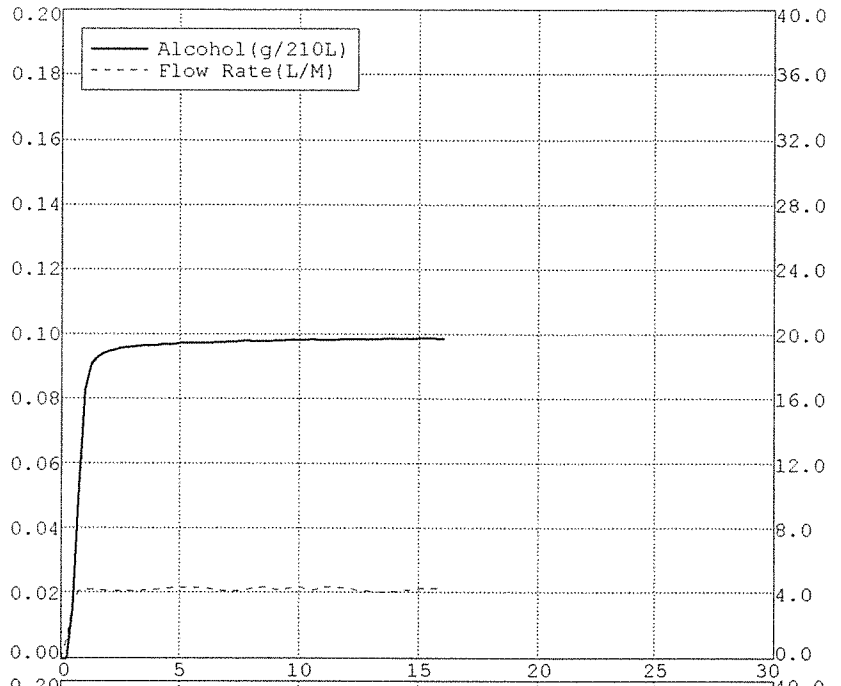

SUPERVISOR TEST

AUBURN CITY  
 POLICE DEPT  
 DATAMASTER dmt: 105406

Date: 10/01/2020

OPERATOR NAME:  
 GREGORY D GILFUS  
 Permit #: 30728  
 Operator Agency/Dept: AUBURN CITY PD  
 Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:40
INTERNAL STANDARD	VERIFIED	07:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:41
BLANK TEST	0.00	07:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:42
BLANK TEST	0.00	07:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:43
BLANK TEST	0.00	07:44

