

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 10/04/2021

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:35
INTERNAL STANDARD	VERIFIED	11:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:36
BLANK TEST	0.00	11:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:37
BLANK TEST	0.00	11:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:38
BLANK TEST	0.00	11:39

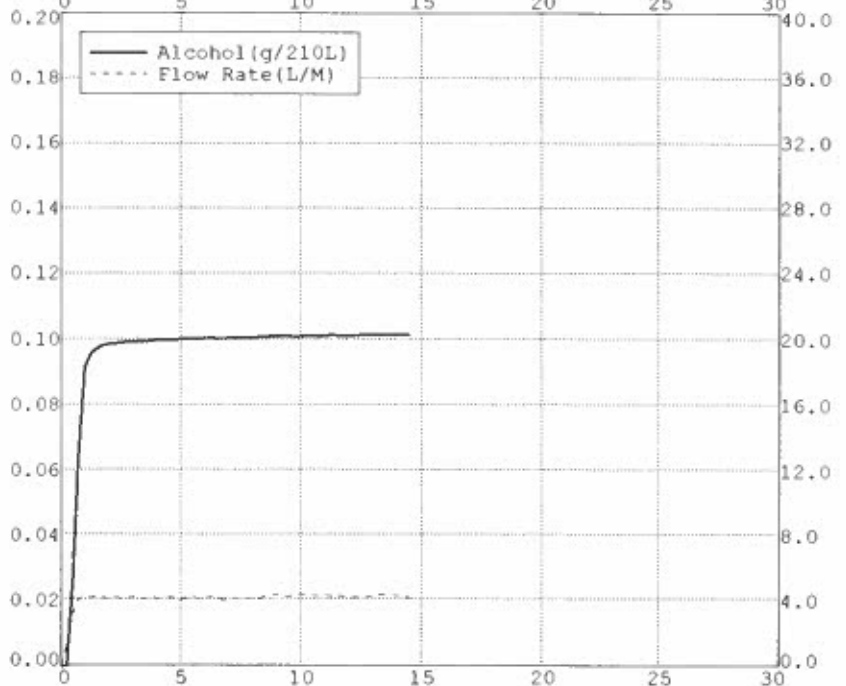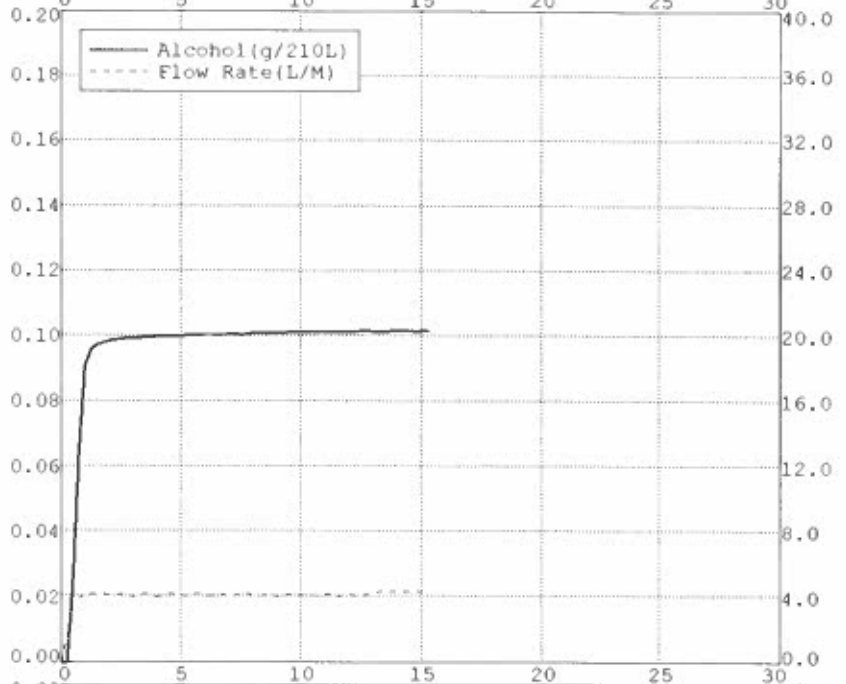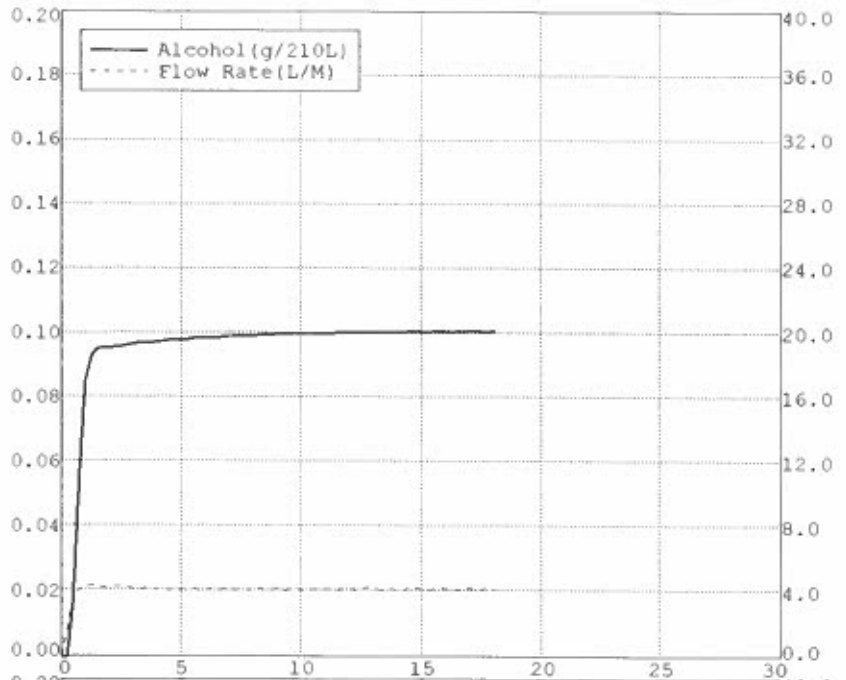

SOLUTION CHANGE

AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 10/04/2021

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:20
INTERNAL STANDARD	VERIFIED	14:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:21
BLANK TEST	0.00	14:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:22
BLANK TEST	0.00	14:23
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	14:23
BLANK TEST	0.00	14:24

