

SOLUTION CHANGE




AUBURN CITY  
 POLICE DEPT  
 DATAMASTER dmt: 105406

Date: 11/01/2021

OPERATOR NAME:  
 GREGORY D GILFUS  
 Permit #: 30728  
 Operator Agency/Dept: AUBURN CITY PD  
 Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:14
INTERNAL STANDARD	VERIFIED	08:14
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:15
BLANK TEST	0.00	08:15
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	08:16
BLANK TEST	0.00	08:17
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	08:17
BLANK TEST	0.00	08:18

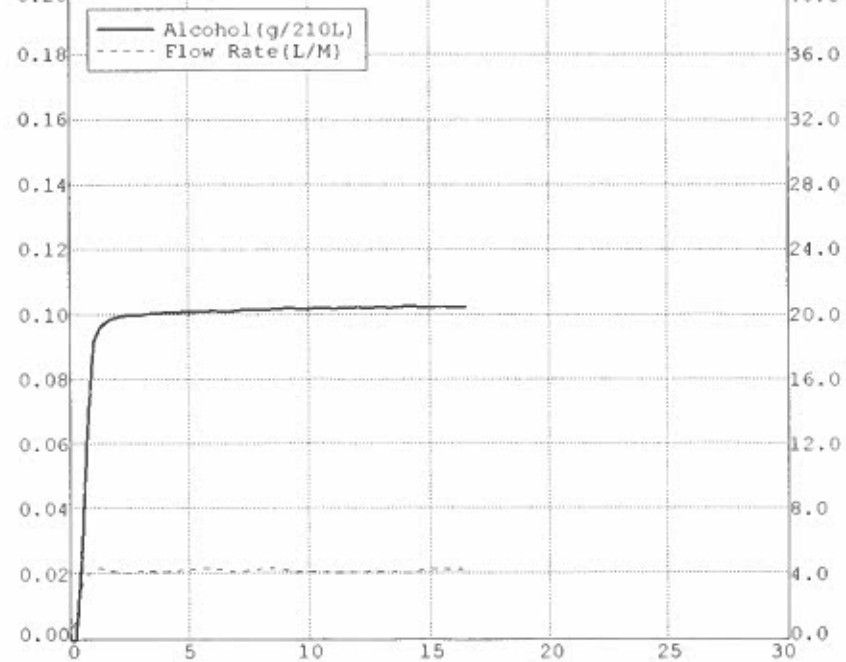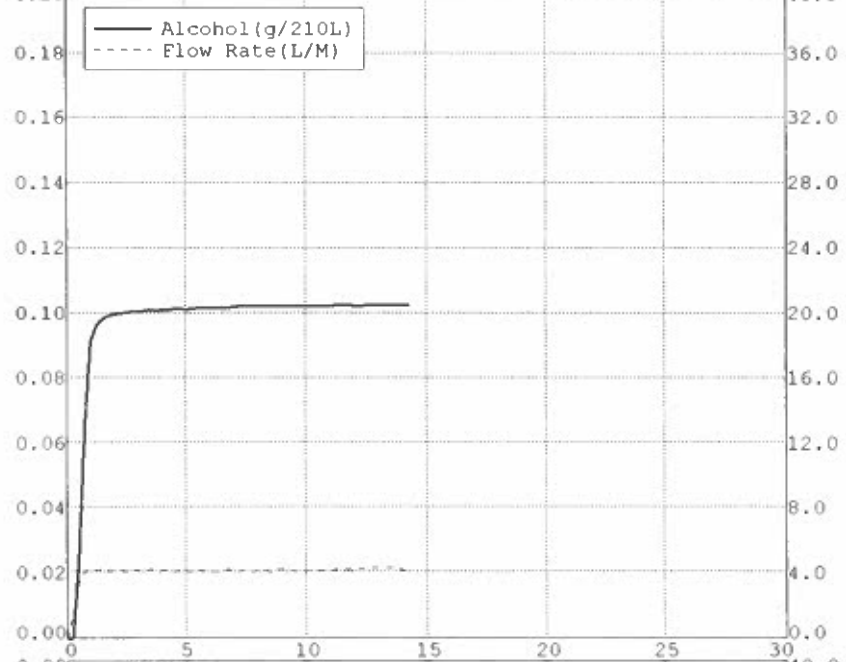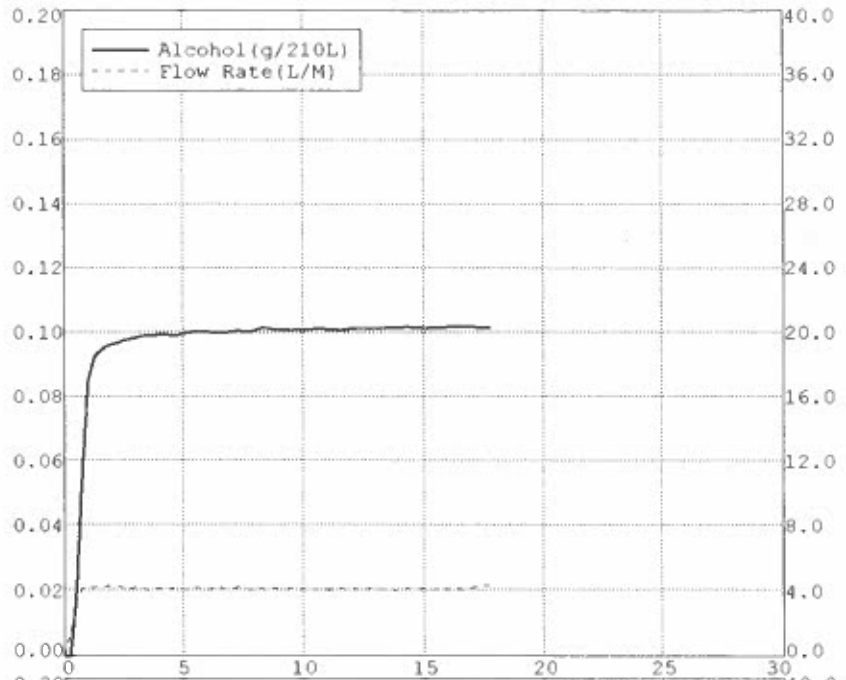

SUPERVISOR TEST

AUBURN CITY  
 POLICE DEPT  
 DATAMASTER dmt: 105406

Date: 11/01/2021

OPERATOR NAME:  
 GREGORY D GILFUS  
 Permit #: 30728  
 Operator Agency/Dept: AUBURN CITY PD  
 Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:48
INTERNAL STANDARD	VERIFIED	07:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:48
BLANK TEST	0.00	07:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:50
BLANK TEST	0.00	07:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:51
BLANK TEST	0.00	07:52

