

SUPERVISOR TEST




AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 11/01/2023

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:20
INTERNAL STANDARD	VERIFIED	08:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:21
BLANK TEST	0.00	08:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:22
BLANK TEST	0.00	08:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:23
BLANK TEST	0.00	08:24

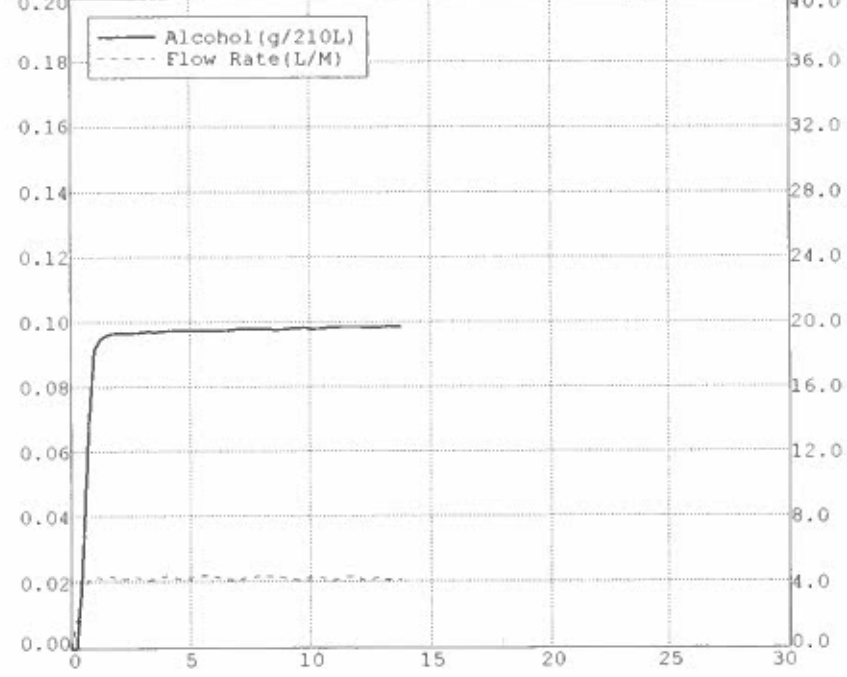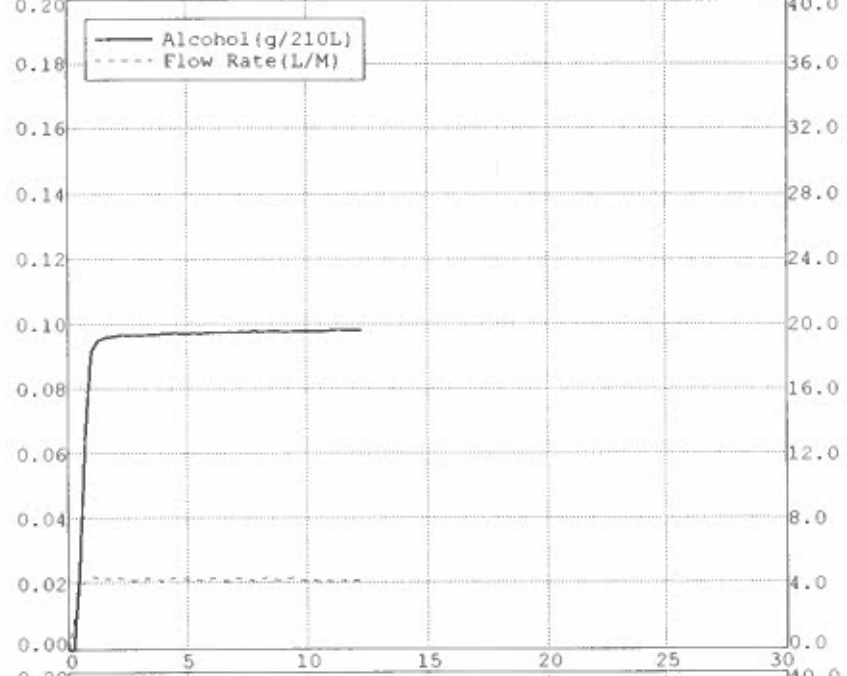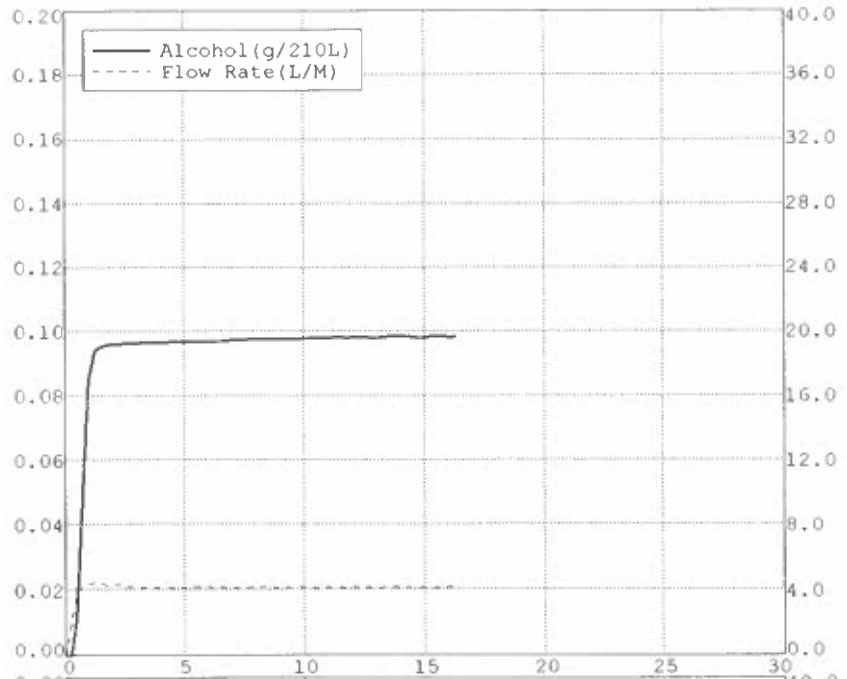

SOLUTION CHANGE

AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 11/01/2023

OPERATOR NAME: *GD*  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:00
INTERNAL STANDARD	VERIFIED	09:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:01
BLANK TEST	0.00	09:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:02
BLANK TEST	0.00	09:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:03
BLANK TEST	0.00	09:04

