

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 12/01/2021

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:02
INTERNAL STANDARD	VERIFIED	08:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:02
BLANK TEST	0.00	08:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:03
BLANK TEST	0.00	08:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:05
BLANK TEST	0.00	08:06

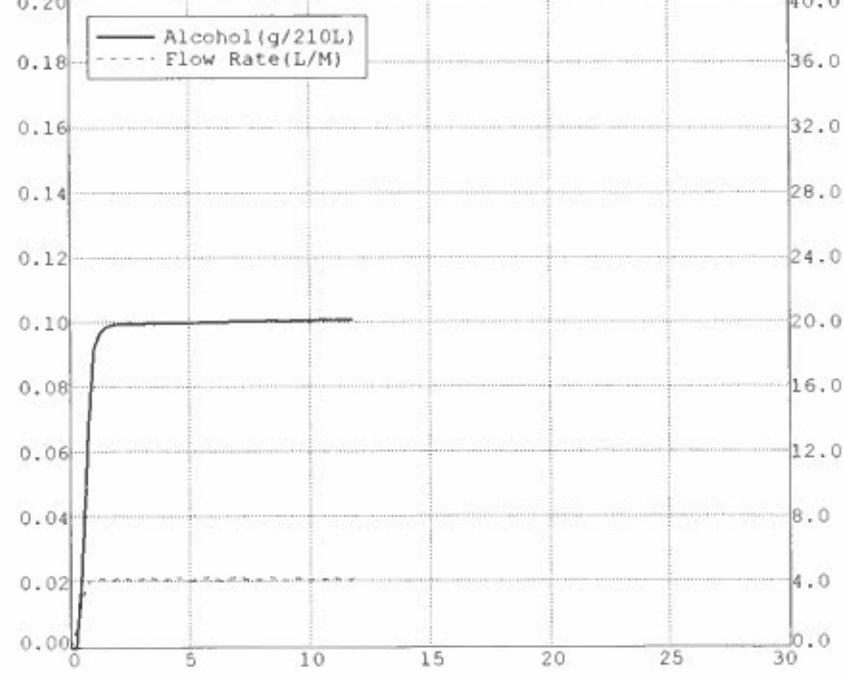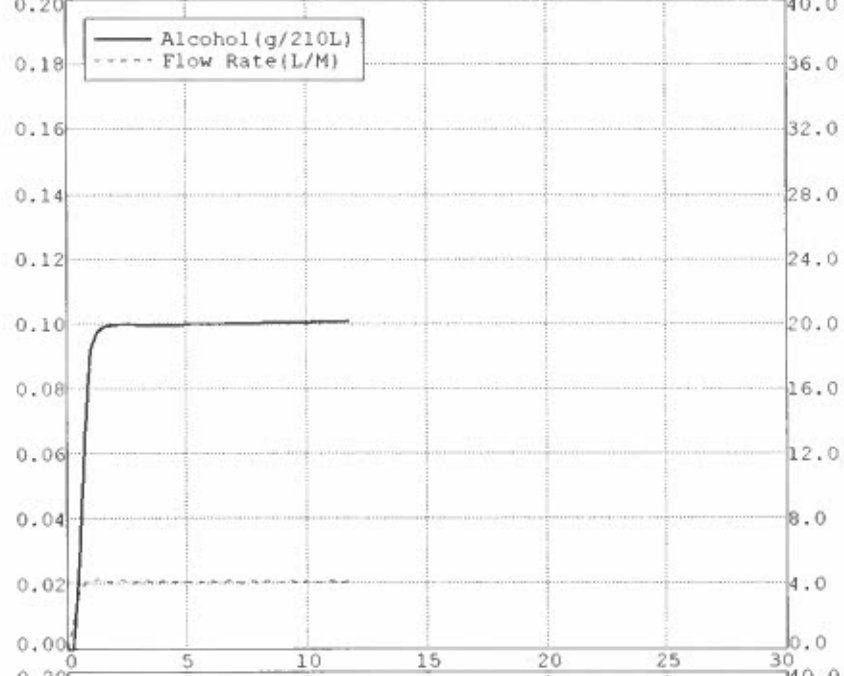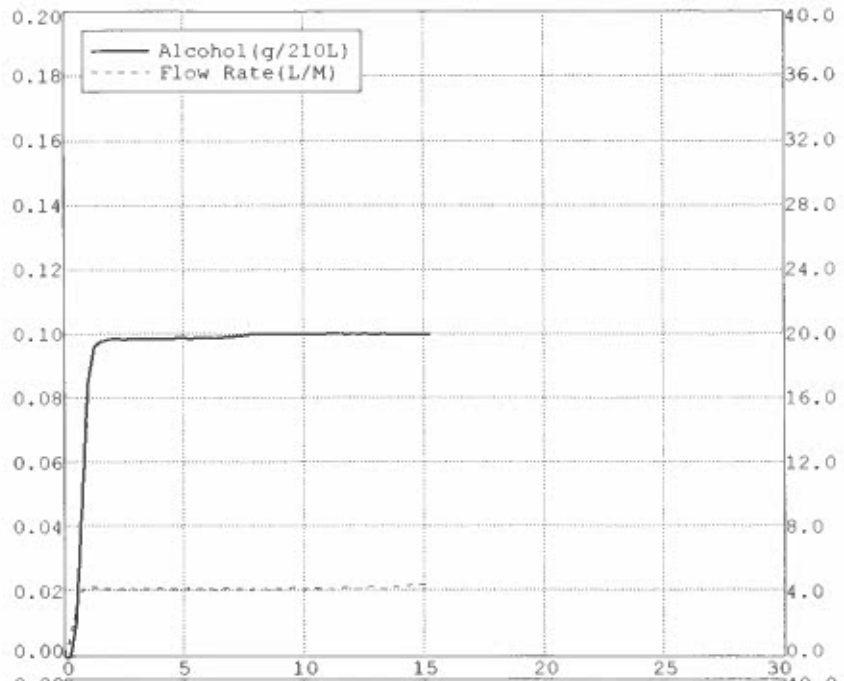

SOLUTION CHANGE

AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 12/01/2021

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:42
INTERNAL STANDARD	VERIFIED	09:42
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:42
BLANK TEST	0.00	09:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:44
BLANK TEST	0.00	09:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:45
BLANK TEST	0.00	09:46

