

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 12/01/2023

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:16
INTERNAL STANDARD	VERIFIED	13:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:17
BLANK TEST	0.00	13:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:18
BLANK TEST	0.00	13:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:19
BLANK TEST	0.00	13:20

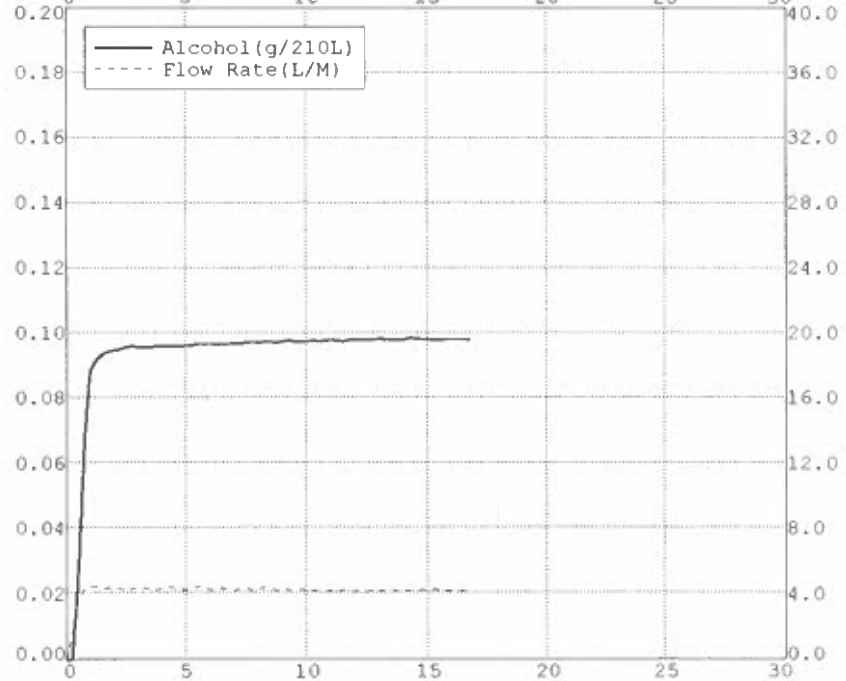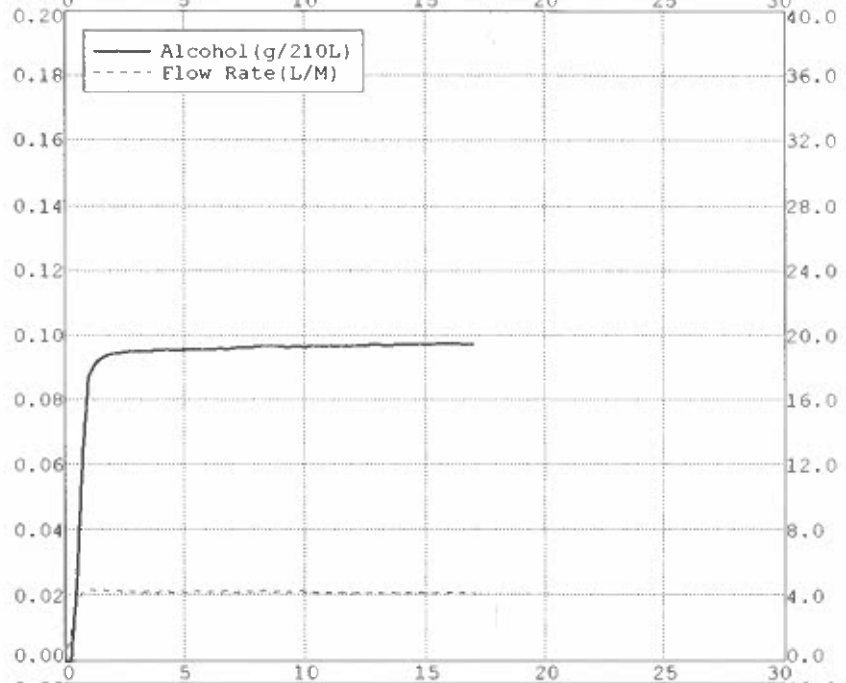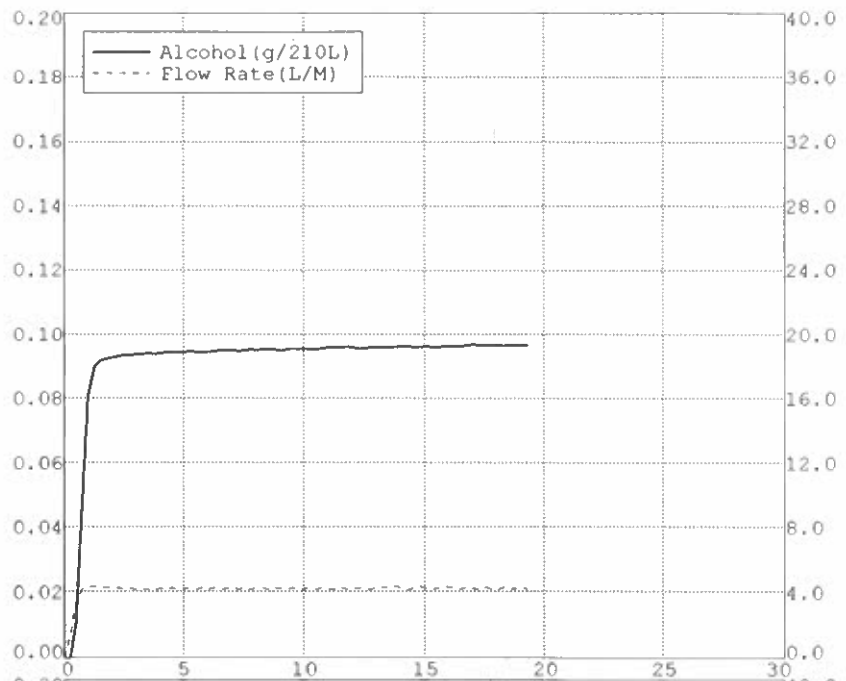

SOLUTION CHANGE

AUBURN CITY
 POLICE DEPT
 DATAMASTER dmt: 105406

Date: 12/01/2023

OPERATOR NAME:
 GREGORY D GILFUS
 Permit #: 30728
 Operator Agency/Dept: AUBURN CITY PD
 Reference Standard #: 23350

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:53
INTERNAL STANDARD	VERIFIED	13:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:53
BLANK TEST	0.00	13:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:54
BLANK TEST	0.00	13:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:56
BLANK TEST	0.00	13:56

