

SUPERVISOR TEST




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 01/03/2022

OPERATOR NAME: GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:23
INTERNAL STANDARD	VERIFIED	07:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:23
BLANK TEST	0.00	07:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:24
BLANK TEST	0.00	07:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:26
BLANK TEST	0.00	07:27

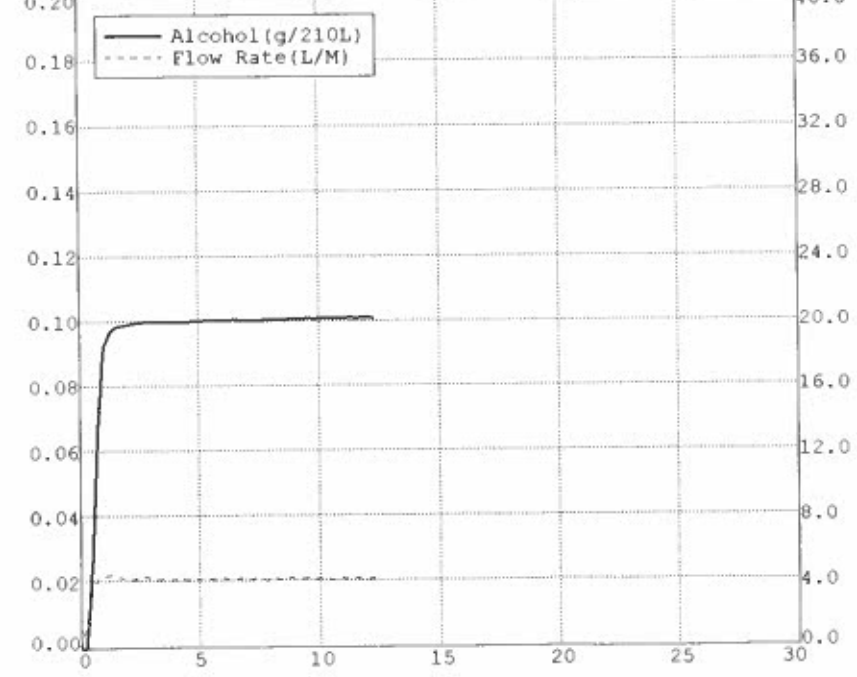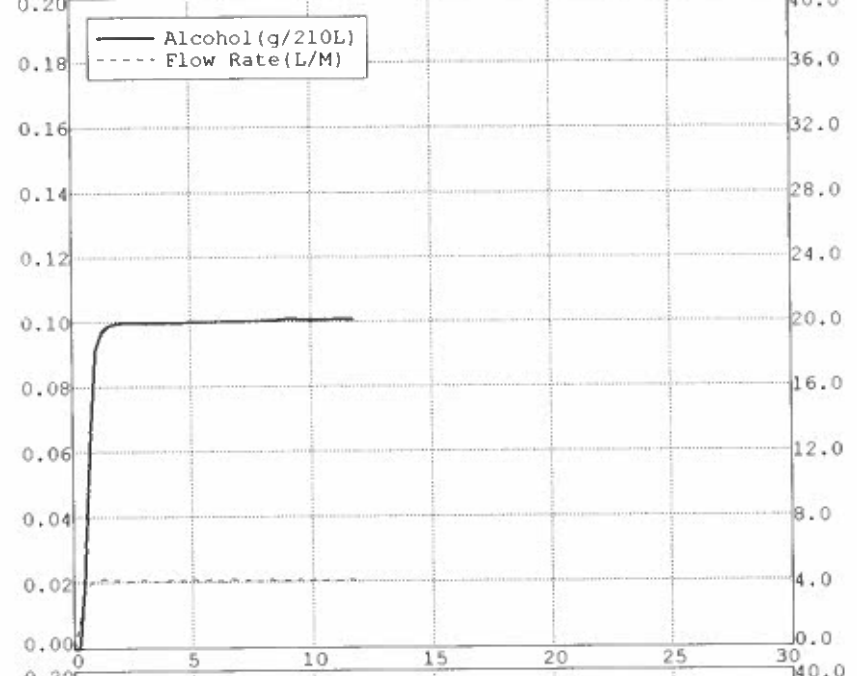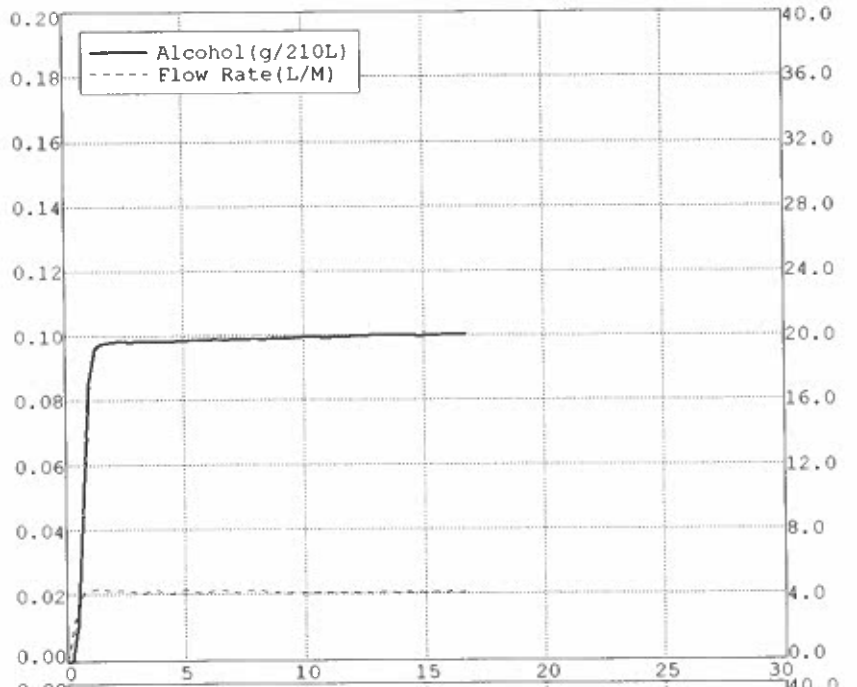

SOLUTION CHANGE

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 01/03/2022

OPERATOR NAME: GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:34
INTERNAL STANDARD	VERIFIED	09:34
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:35
BLANK TEST	0.00	09:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:36
BLANK TEST	0.00	09:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:37
BLANK TEST	0.00	09:38

