

SOLUTION CHANGE




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 02/03/2020

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:45
INTERNAL STANDARD	VERIFIED	09:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:46
BLANK TEST	0.00	09:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:47
BLANK TEST	0.00	09:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:48
BLANK TEST	0.00	09:49

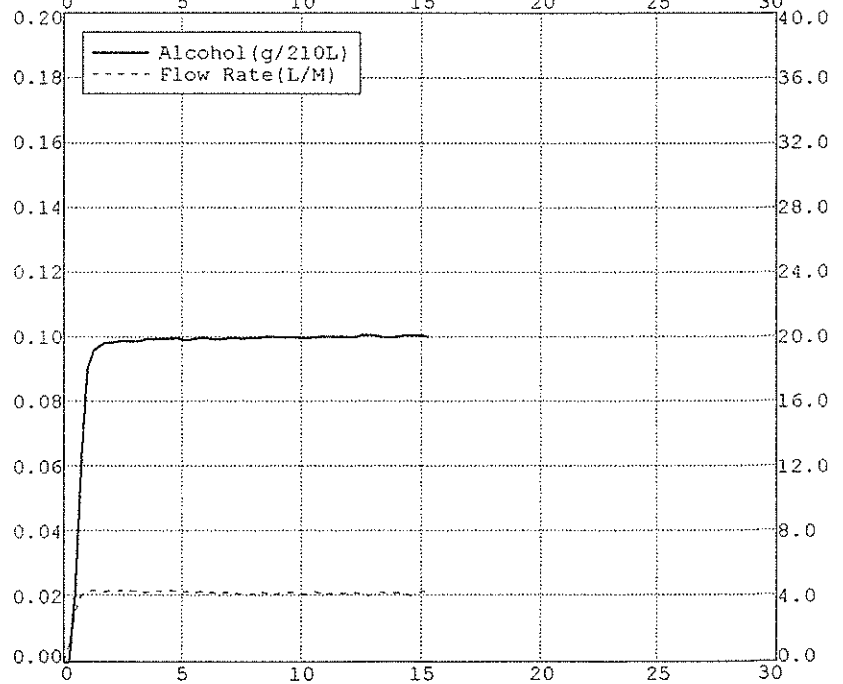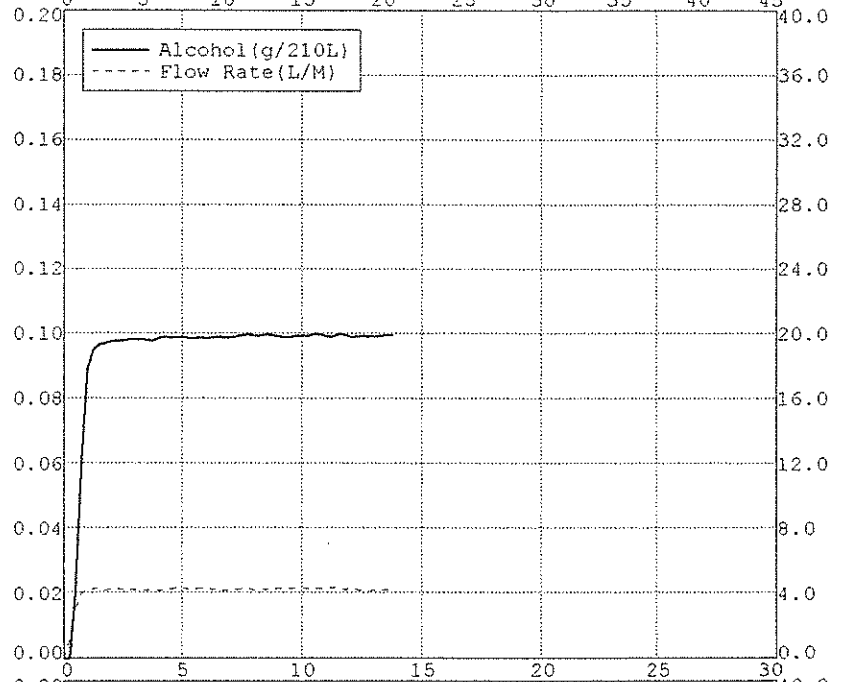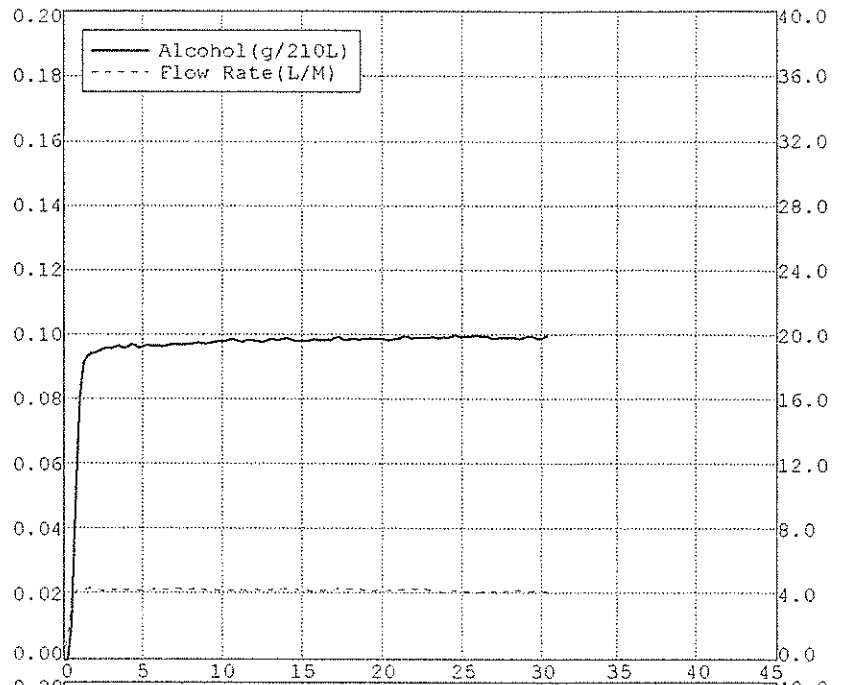

SUPERVISOR TEST

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 02/03/2020

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:44
INTERNAL STANDARD	VERIFIED	07:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:45
BLANK TEST	0.00	07:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:46
BLANK TEST	0.00	07:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:47
BLANK TEST	0.00	07:48

