

SUPERVISOR TEST




AUBURN CITY  
 POLICE DEPT  
 DATAMASTER dmt: 105406

Date: 03/02/2020

OPERATOR NAME:  
 GREGORY D GILFUS *GW*  
 Permit #: 30728  
 Operator Agency/Dept: AUBURN CITY PD  
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:11
INTERNAL STANDARD	VERIFIED	07:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:11
BLANK TEST	0.00	07:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:12
BLANK TEST	0.00	07:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:13
BLANK TEST	0.00	07:14

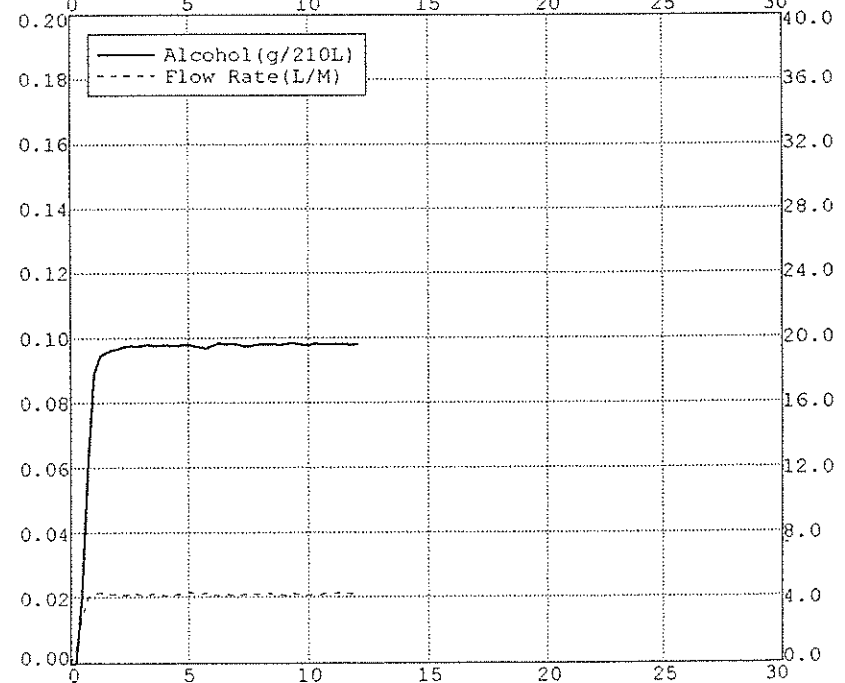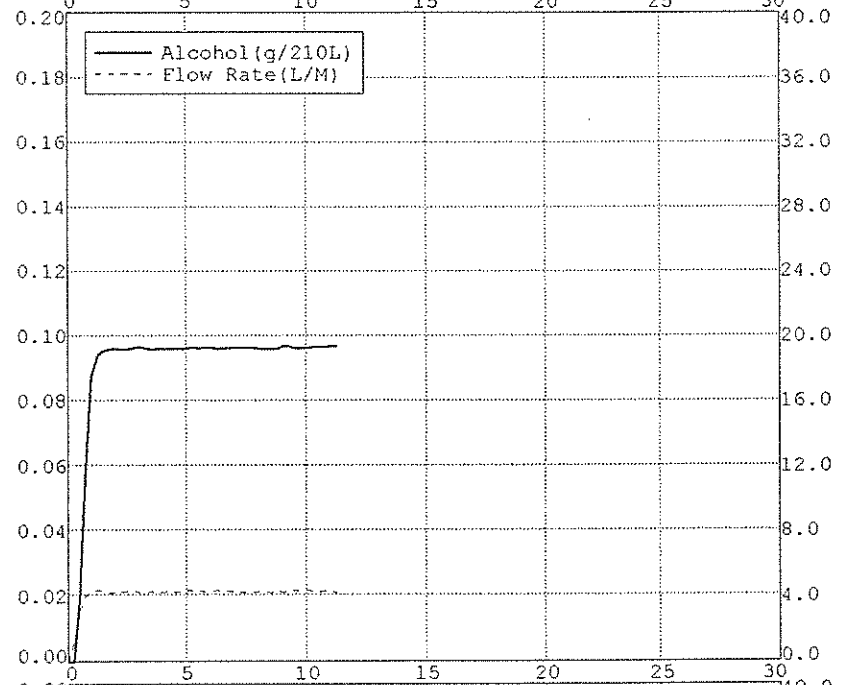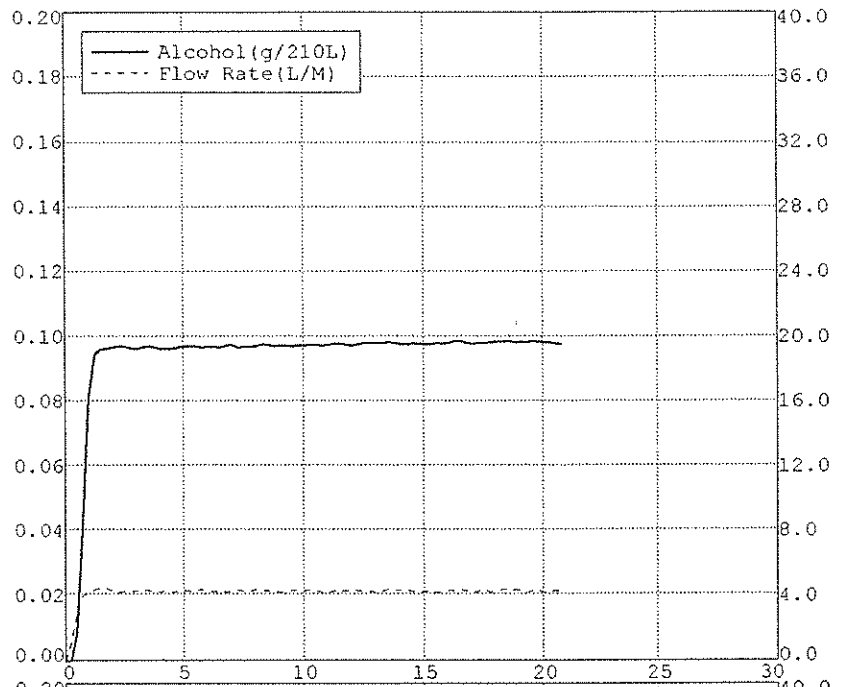

SOLUTION CHANGE

AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 03/02/2020

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:44
INTERNAL STANDARD	VERIFIED	07:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:44
BLANK TEST	0.00	07:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:46
BLANK TEST	0.00	07:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:47
BLANK TEST	0.00	07:48

