

SUPERVISOR TEST




AUBURN CITY  
POLICE DEPT  
MATAMASTER dmt: 105406

Date: 03/30/2020

OPERATOR NAME: GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:10
INTERNAL STANDARD	VERIFIED	11:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:11
BLANK TEST	0.00	11:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:12
BLANK TEST	0.00	11:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:13
BLANK TEST	0.00	11:14

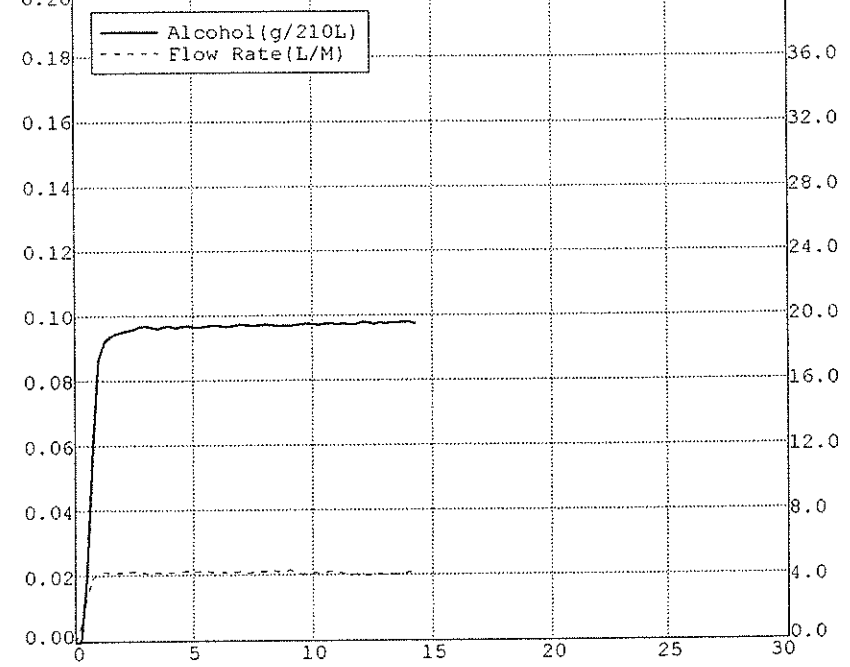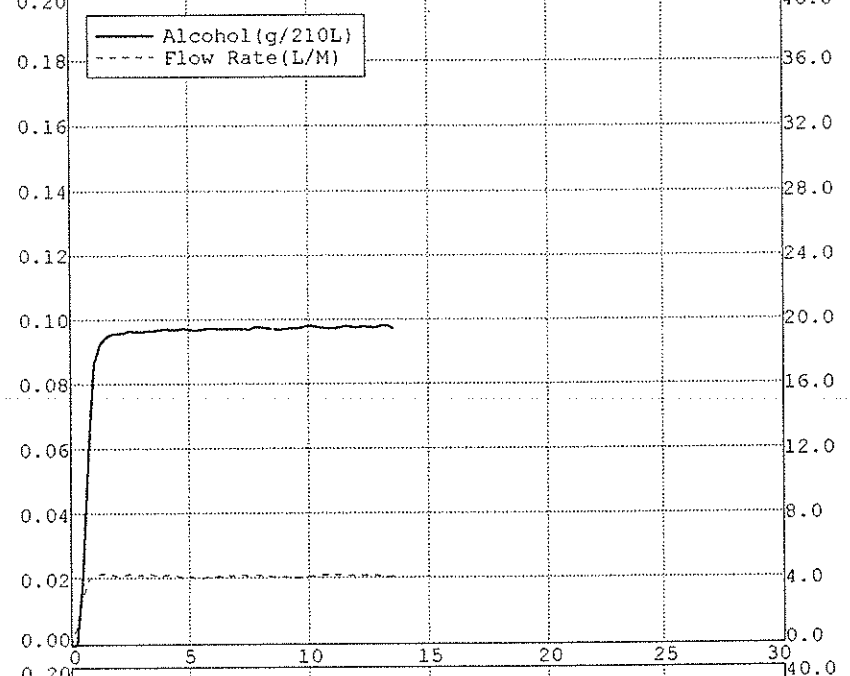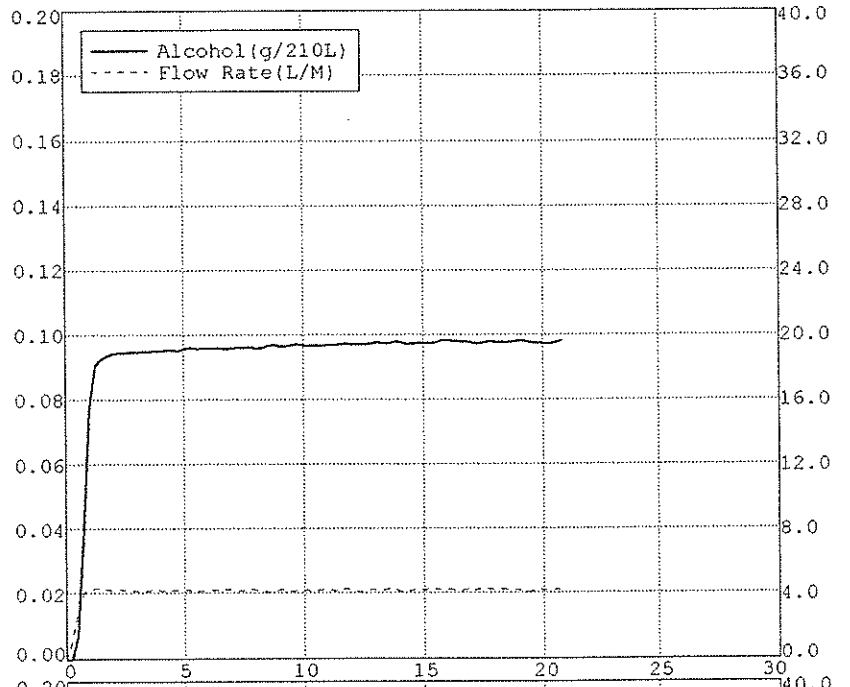

SOLUTION CHANGE

AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 04/01/2020

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:32
INTERNAL STANDARD	VERIFIED	12:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:33
BLANK TEST	0.00	12:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:34
BLANK TEST	0.00	12:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:35
BLANK TEST	0.00	12:36

