

SUPERVISOR TEST




AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 06/01/2020

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:48
INTERNAL STANDARD	VERIFIED	07:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:49
BLANK TEST	0.00	07:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:50
BLANK TEST	0.00	07:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:51
BLANK TEST	0.00	07:52

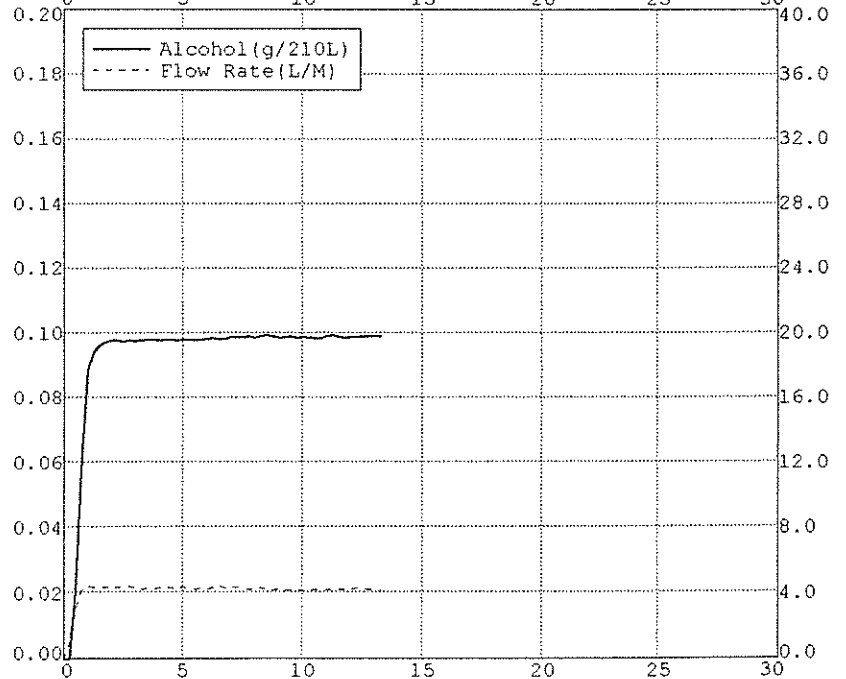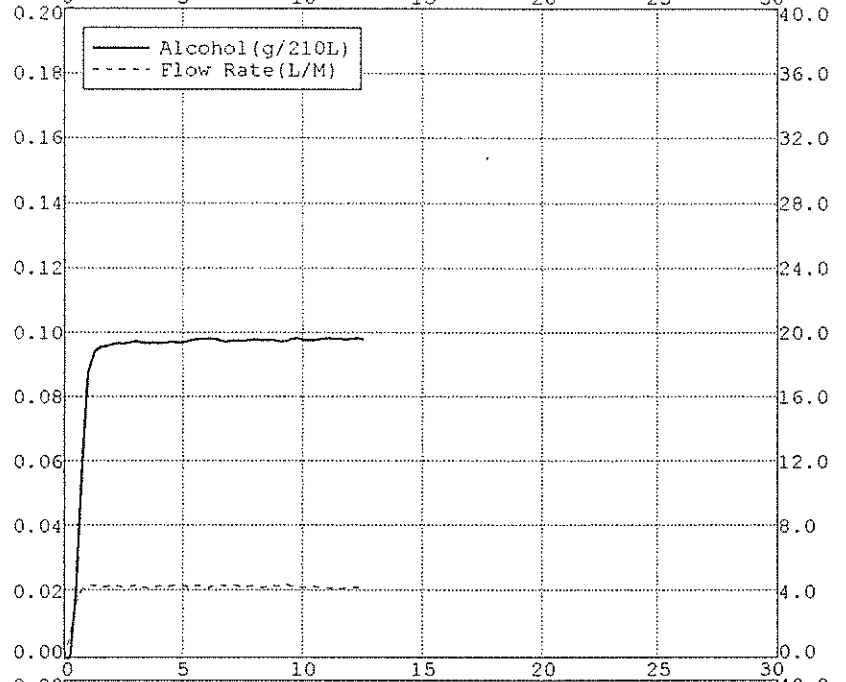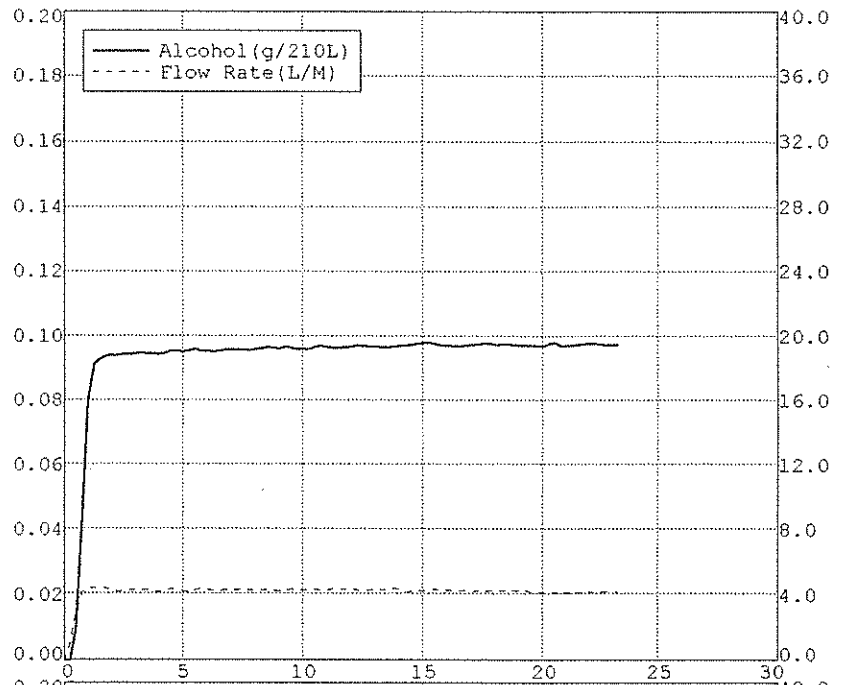

SOLUTION CHANGE

AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 06/01/2020

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:58
INTERNAL STANDARD	VERIFIED	08:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:59
BLANK TEST	0.00	09:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:00
BLANK TEST	0.00	09:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:01
BLANK TEST	0.00	09:02

