

SOLUTION CHANGE




AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 07/01/2020

OPERATOR NAME:
GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:17
INTERNAL STANDARD	VERIFIED	08:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:18
BLANK TEST	0.00	08:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:19
BLANK TEST	0.00	08:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:20
BLANK TEST	0.00	08:21

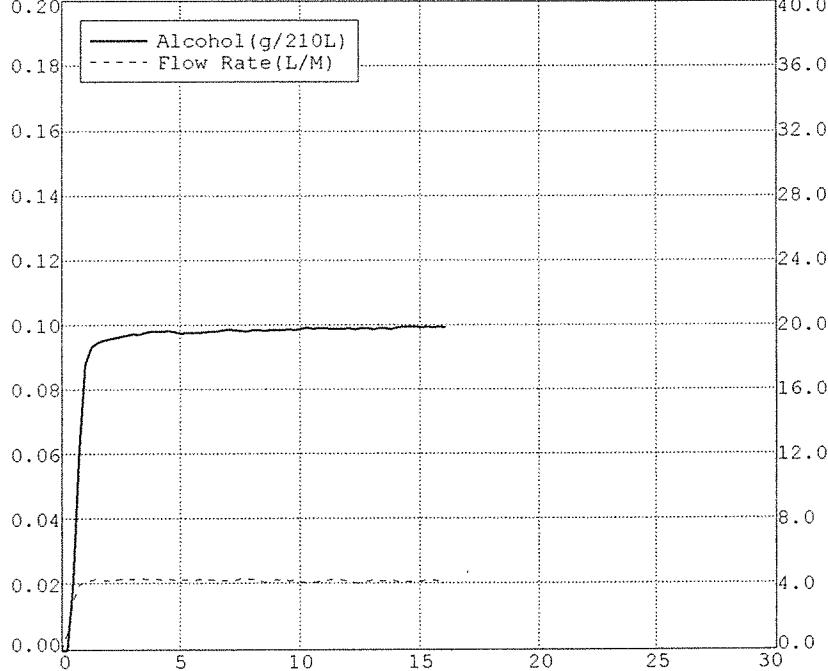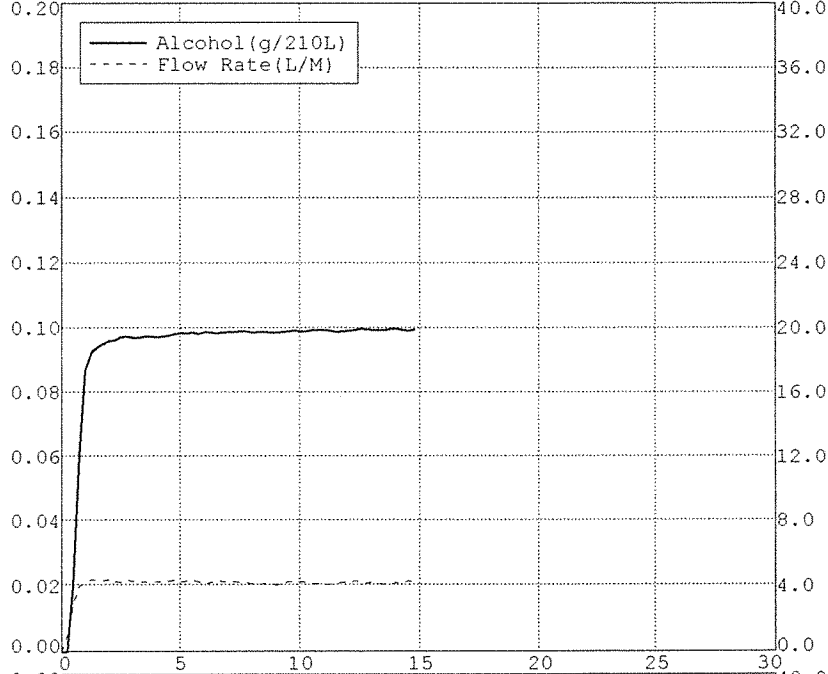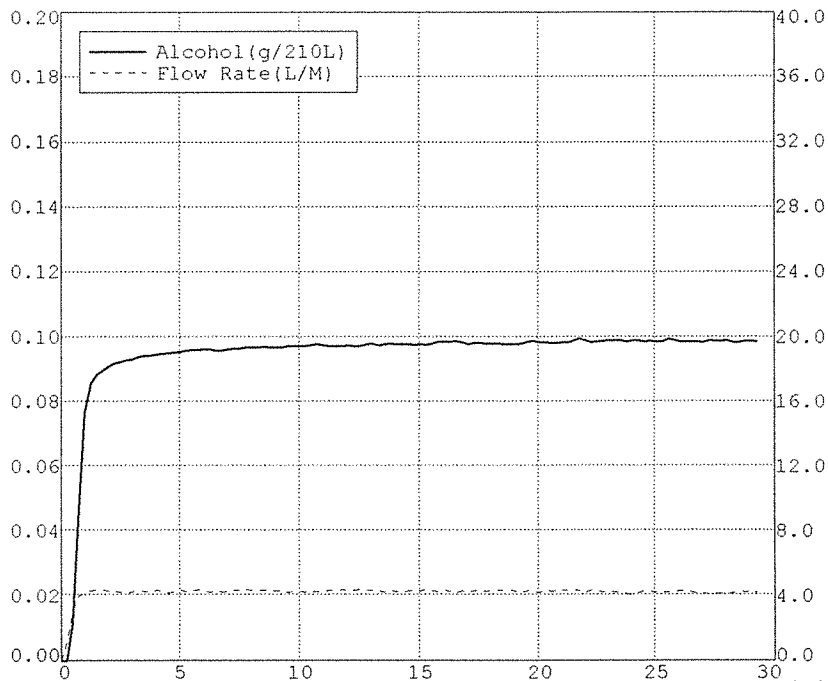

SUPERVISOR TEST

AUBURN CITY
POLICE DEPT
DATAMASTER dmt: 105406

Date: 07/01/2020

OPERATOR NAME: GREGORY D GILFUS
Permit #: 30728
Operator Agency/Dept: AUBURN CITY PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:35
INTERNAL STANDARD	VERIFIED	07:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:36
BLANK TEST	0.00	07:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:37
BLANK TEST	0.00	07:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	07:38
BLANK TEST	0.00	07:39

