

SOLUTION CHANGE



AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 11/06/2020

OPERATOR NAME:  
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 20340

Nominal = 0.10 g/210L


BLANK TEST	0.00	08:13
INTERNAL STANDARD	VERIFIED	08:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:14
BLANK TEST	0.00	08:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:15
BLANK TEST	0.00	08:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:16
BLANK TEST	0.00	08:17

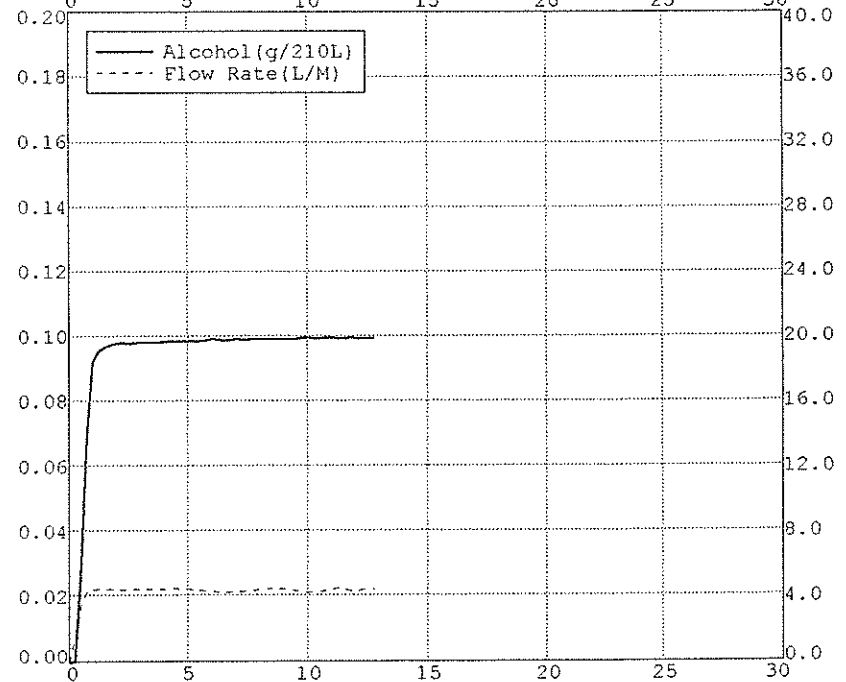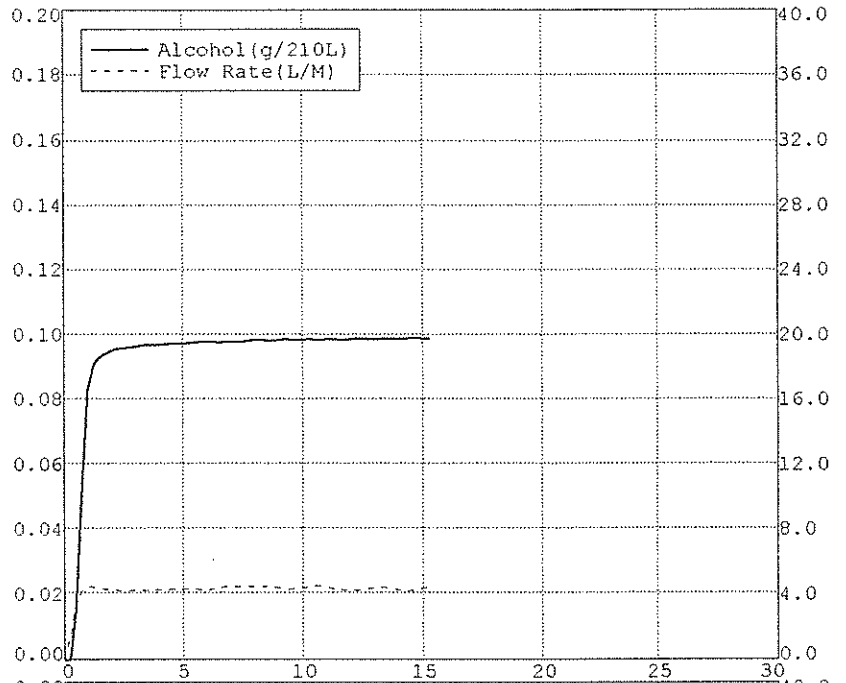

SUPERVISOR TEST

AUBURN CITY  
POLICE DEPT  
DATAMASTER dmt: 105406

Date: 11/06/2020

OPERATOR NAME:   
GREGORY D GILFUS  
Permit #: 30728  
Operator Agency/Dept: AUBURN CITY PD  
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:42
INTERNAL STANDARD	VERIFIED	07:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:43
BLANK TEST	0.00	07:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:44
BLANK TEST	0.00	07:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:45
BLANK TEST	0.00	07:46

